
ottobock.

C-Brace Cockpit app.
User guide.

Cockpit App Display

1. Navigation menu
2. Component name
   (Created in Setup App)
3. Switch components
4. MyModes
5. Current selected mode
6. Charge level
7. Display and current mode
8. Connected to component
   Connection interrupted

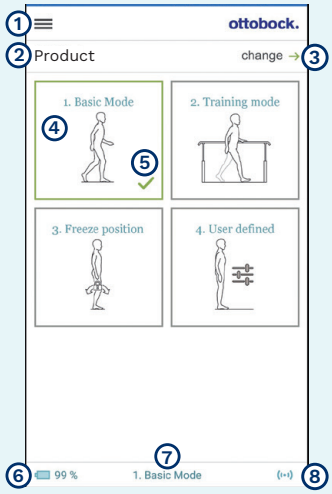

MyModes

Basic Mode
This mode is intended for daily use

Training Mode
Knee flexion is blocked in stance phase, releases in swing phase once release criteria is met

Freeze Position
Knee flexion and extension are blocked in the angle of patient's choice of 0-65°. Deactivate by selecting a different Mode or turning joint on/off

User Defined
Intended for specific motion patterns. Configured by clinician

Parameters in Basic Mode

Stance Flexion Resistance
Resistance against knee flexion when walking down stairs or sitting down

Stance Function (must be enabled by O&P clinician)
The joint is fixed in flexion at an angle of 5-65°

Sitting Function
Minimal extension resistance while seated for easier mobility

Volume of Acoustic Signal
Volume of beep signal for confirmation tones

Pitch of Acoustic Signal
Pitch of beep signal for confirmation tones

Please contact your O&P clinician with further questions.

Navigation Menu

Product
Name of connected component

MyModes
Main menu to switch to MyModes

Settings
Change settings of component

Manage Components
Add or delete components

Imprint/Info
Information/legal notices

Bluetooth® Connection

- C-Brace and Bluetooth® must be turned on
- The device must be connected to the internet
- In the Cockpit app, tap "Add Component" to access Connection Wizard
- Enter Bluetooth® PIN (card with SN/PIN included at fitting)
- A successful connection will be indicated by 3 beep signals and a symbol in the bottom corner
- For troubleshooting, please see the C-Brace IFU

Scan the QR code for Therapy Exercises

ottobock.com
US: P 800 328 4058 | F 800 962 2549
CA: P 800 665 3327 | F 800 463 3659

©2025 Otto Bock HealthCare LP · 23755 · 09/25 · Technical changes and printing errors reserved.