

Confirm Setup


Experiment Name: 20220208-1411_full-01
 Instruction Level: Standard
 GEM Check?: Yes
 V(D)J Amplification?: No
 qPCR Setup?: No
 Pooling?: No
 cDNA Cycles: 16

Sample ID	SI Plate	Target Cell #	Expression
1 a	A4	500-2000	High
2 b	B4	500-2000	High

Please review these Setup selections (experiment name, inputs, and sample information), before proceeding on to the next stage of the run.

BACK

CONFIRM



SC5'GEX >

Setup >

Load >

Run >

Complete

Gather Items

Gather Reagents >

Get Started

1. Retrieve the listed consumables:

Item	Qty
Nuclease-free Water	10 ml
Ethanol, Pure (200 Proof, anhydrous)	40 ml
Hamilton	
Comfort Lids	6
50 µl Black CO-RE Pipette Tips, with filter	1 rack
300 µl Black CO-RE Pipette Tips, with filter	2 racks
Reagent Reservoirs, 60 ml	3
Eppendorf	
Semi Skirted Plate, 96 well	1
Full Skirted Plate, 96 well	1
Thermo Fisher Scientific	
MicroAmp 8-tube strips, 0.2 ml	2
10x Genomics	
Chromium Next GEM Chip K Automated Single Cell Kit <i>Partitioning Oil, 50% Glycerol, Chip K (keep sealed)</i>	1

CANCEL

SCAN

CONFIRM

SC5'GEX >

Setup >

Load >

Run >

Complete

< Gather Items

Gather Reagents

Prep Modules >

Get Started


1. Retrieve the listed Chromium Next GEM Automated Single Cell 5' Kit v2 items:

Box Label, Item	Temp, Qty
Library Module 1	4°C
Library Module 1 <i>Black tube strip</i>	1 tube strip/sample
Dynabeads MyOne SILANE	1 tube/run
Library Module 2	-20°C
Library Module 2 <i>Gray tube strip</i>	1 tube strip/sample
Library Module 3	-20°C
Library Module 3 <i>White tube strip</i>	1 tube strip/sample
Poly-dT RT Primer	1 tube/run
Sample Index Plate (SI Plate)	-20°C
Dual Index Plate TT Set A	1 plate
Single Cell 5' Gel Beads v2	-80°C
Gel Bead Strip/s	1 tube/sample

CANCEL

SCAN

CONFIRM



SC5'GEX >

Setup >

Load >

Run >

Complete

< Gather Reagents

Prep Modules

Remove Carriers >

Start Timer

1. Thaw the listed reagents for **30 min**:

Temp, Location

37°C, Benchtop Thermal Cycler (*lid temperature 50°C*)

Library Module 1, Black tube strip
After 15 min, vortex & return

4°C, Storage

Library Module 3, White tube strip

Room Temperature, Off-Deck Workspace

Library Module 2, Gray tube strip

Dynabeads

Gel Beads

Poly-dT RT Primer

SI Plate

2. Process to next screen while reagents thaw.

CANCEL

SCAN 

CONFIRM

SC5'GEX >

Setup >

Load >

Run >

Complete

< Prep Modules

Remove Carriers


Load Consumables >

Remove Carriers From Deck

During Reagent Thaw

1. Open Front Panel.
2. Slide out Carriers 3, 4, and 5 from the deck completely and place on an off-deck workspace.

Carriers: ① ② ③ ④ ⑤

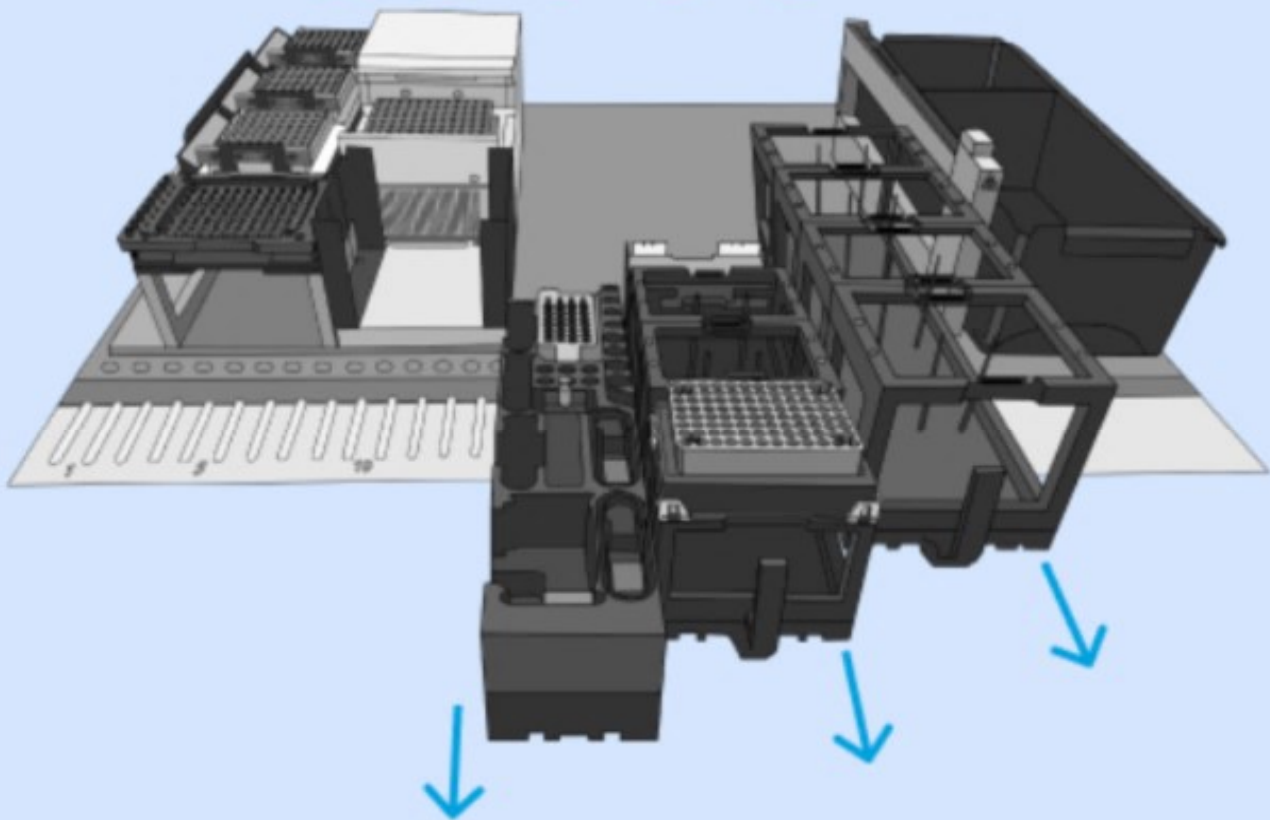

CANCEL

SCAN 

CONFIRM

SC5'GEX > Setup > **Load** > Run > Complete

< Remove Carriers



Load Consumables

Load SI Plate >

Carrier Loading
During Reagent Thaw

1. Load consumables into corresponding locations in Carriers 2, 4, and 5:

Item	Qty	Location
Comfort Lids	6 ea	Zone 4
50 µl Pipette Tips <i>Barcodes face right in carrier</i>	1 ea	Zone 6
Semi Skirted Plate <i>A1 top left</i>	1 ea	Zone 7
300 µl Pipette Tips <i>Barcodes face right in carrier</i>	2 ea	Zone 8

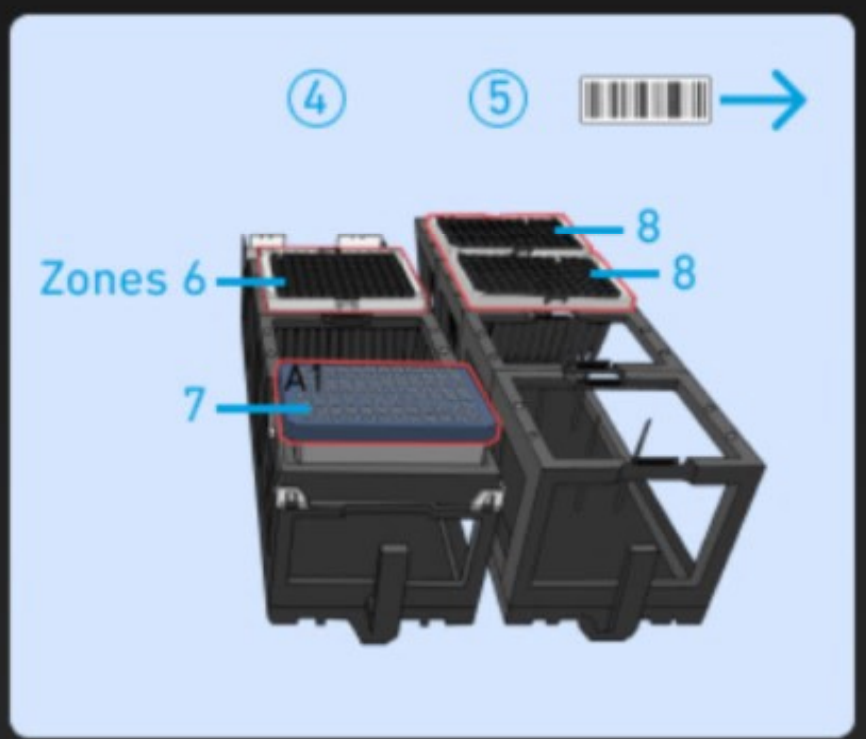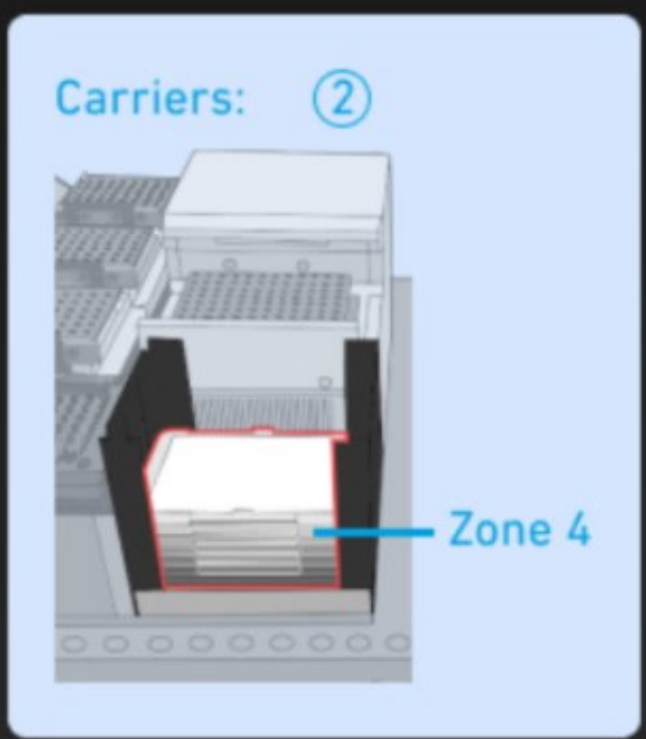

CANCEL

SCAN

CONFIRM