

USER GUIDE

# Chromium Next GEM Single Cell Multiome ATAC + Gene Expression



FOR USE WITH

**Chromium Next GEM Single Cell Multiome ATAC + Gene Expression Reagent Bundle, 16 rxns PN-1000283, includes:**

- Chromium Next GEM Single Cell Multiome ATAC Kit A, 16 rxns PN-1000280
- Chromium Next GEM Single Cell Multiome Reagent Kit A, 16 rxns PN-1000282
- Library Construction Kit, 16 rxns PN-1000190

**Chromium Next GEM Single Cell Multiome ATAC + Gene Expression Reagent Bundle, 4 rxns PN-1000285, includes:**

- Chromium Next GEM Single Cell Multiome ATAC Kit A, 4 rxns PN-1000281
- Chromium Next GEM Single Cell Multiome Reagent Kit A, 4 rxns PN-1000284
- Library Construction Kit B, 4 rxns PN-1000279

**Chromium Next GEM Chip J Single Cell Kit, 48 rxns PN-1000234**

**Chromium Next GEM Chip J Single Cell Kit, 16 rxns PN-1000230**

**Single Index Kit N Set A, 96 rxns PN-1000212**

**Dual Index Kit TT Set A, 96 rxns PN-1000215**

Next GEM reagents are specific to Next GEM products and should not be used interchangeably with non-Next GEM reagents.

## Notices

### Document Number

CG000338 • Rev D

### Legal Notices

©2021 10x Genomics, Inc. (10x Genomics). All rights reserved. Duplication and/or reproduction of all or any portion of this document without the express written consent of 10x Genomics, is strictly forbidden. Nothing contained herein shall constitute any warranty, express or implied, as to the performance of any products described herein. Any and all warranties applicable to any products are set forth in the applicable terms and conditions of sale accompanying the purchase of such product. 10x Genomics provides no warranty and hereby disclaims any and all warranties as to the use of any third-party products or protocols described herein. The use of products described herein is subject to certain restrictions as set forth in the applicable terms and conditions of sale accompanying the purchase of such product. A non-exhaustive list of 10x Genomics' marks, many of which are registered in the United States and other countries can be viewed at: [www.10xgenomics.com/trademarks](http://www.10xgenomics.com/trademarks). 10x Genomics may refer to the products or services offered by other companies by their brand name or company name solely for clarity, and does not claim any rights in those third-party marks or names. 10x Genomics products may be covered by one or more of the patents as indicated at: [www.10xgenomics.com/patents](http://www.10xgenomics.com/patents). The use of products described herein is subject to 10x Genomics Terms and Conditions of Sale, available at [www.10xgenomics.com/legal-notices](http://www.10xgenomics.com/legal-notices), or such other terms that have been agreed to in writing between 10x Genomics and user. All products and services described herein are intended FOR RESEARCH USE ONLY and NOT FOR USE IN DIAGNOSTIC PROCEDURES.

Notice to Customer: The listed products and their use are the subject of United States Patent Nos. 6,159,736, and 6,294,385, European Patent No. 1115856 and related patents and patent applications licensed from the Wisconsin Alumni Research Foundation.

### Instrument & Licensed Software Updates Warranties

Updates to existing Instruments and Licensed Software may be required to enable customers to use new or existing products. In the event of an Instrument failure resulting from an update, such failed Instrument will be replaced or repaired in accordance with the 10x Limited Warranty, Assurance Plan or service agreement, only if such Instrument is covered by any of the foregoing at the time of such failure. Instruments not covered under a current 10x Limited Warranty, Assurance Plan or service agreement will not be replaced or repaired.

### Support

Email: [support@10xgenomics.com](mailto:support@10xgenomics.com)

10x Genomics

6230 Stoneridge Mall Road

Pleasanton, CA 94588 USA

---

## Document Revision Summary

<b>Document Number</b>	CG000338
<b>Title</b>	Chromium Next GEM Single Cell Multiome ATAC + Gene Expression User Guide
<b>Revision</b>	Rev C to Rev D
<b>Revision Date</b>	May 2021

### Specific Changes:

- NextSeq 1000/2000 included as a compatible sequencer (page 68-70).

### General Changes:

- Updated for general minor consistency of language and terms throughout.

---

# Table of Contents

Introduction	6
Chromium Next GEM Single Cell Multiome Reagents	7
Chromium Accessories	13
Recommended Thermal Cyclers	13
Additional Kits, Reagents & Equipment	14
Protocol Steps & Timing	16
Stepwise Objectives	17
Tips & Best Practices	21
Step 1	27
Transposition	28
1.1 Prepare Transposition Mix	30
1.2 Isothermal Incubation	30
Step 2	31
GEM Generation & Barcoding	32
2.1 Prepare Master Mix	33
2.2 Load Chromium Next GEM Chip J	34
2.3 Run the Chromium Controller	35
2.4 Transfer GEMs	35
2.5 GEM Incubation	36
2.6 Quenching Reaction	36
Step 3	37
Post GEM Incubation Cleanup	38
3.1 Post GEM Incubation Cleanup – Dynabeads	39
3.2 Post GEM Incubation Cleanup – SPRIselect	41
Step 4	42
Pre-Amplification PCR	43
4.1 Prepare Pre-Amplification Mix	44
4.2 Pre-Amplification PCR	44
4.3 Pre-Amplification SPRI Cleanup	45

---

Step 5	47
ATAC Library Construction	48
5.1 Sample Index PCR	49
5.2 Post Sample Index Double Sided Size Selection – SPRIselect	50
5.3 Post Library Construction QC	51
Step 6	52
cDNA Amplification	53
6.1 cDNA Amplification	54
6.2 cDNA Cleanup – SPRIselect	55
6.3 cDNA QC & Quantification	56
Step 7	57
Gene Expression Library Construction	58
7.1 Fragmentation, End Repair & A-tailing	60
7.2 Post Fragmentation, End Repair & A-tailing Double Sided Size Selection – SPRIselect	61
7.3 Adaptor Ligation	62
7.4 Post Ligation Cleanup – SPRIselect	63
7.5 Sample Index PCR	64
7.6 Post Sample Index PCR Double Sided Size Selection – SPRIselect	65
7.7 Post Library Construction QC	66
Sequencing	67
Troubleshooting	71
GEMs	72
Chromium Controller Errors	74
Appendix	75
Agilent TapeStation Traces	77
LabChip Traces	78
Assay Scheme Overview	79
Sequences	80

# Introduction

Chromium Next GEM Single Cell Multiome ATAC + Gene Expression Reagents

Chromium Accessories

Recommended Thermal Cyclers

Additional Kits, Reagents & Equipment

Protocol Steps & Timing

Stepwise Objectives

## Chromium Next GEM Single Cell Multiome Reagent Kit A, 16 rxns PN-1000282

## Chromium Next GEM Single Cell Multiome GEM Kit A, 16 rxns PN-1000232 (store at -20°C)

## Chromium

## Next GEM Single Cell Multiome GEM Kit A

Store at -20°C

	#	PN
● Barcoding Reagent Mix	1	2000267
● Barcoding Enzyme Mix	1	2000266
● Template Switch Oligo	1	3000228
○ Reducing Agent B	1	2000087
● Cleanup Buffer	2	2000088
● Quenching Agent	1	2000269

10xGenomics.com

10x  
GENOMICS

## Chromium Next GEM Single Cell Multiome Amp Kit A, 16 rxns PN-1000233 (store at -20°C)

## Chromium

## Next GEM Single Cell Multiome Amp Kit A

Store at -20°C

	#	PN
● Pre-Amp Mix	1	2000270
● Pre-Amp Primers	1	2000271
○ Amp Mix	2	2000047
● SI-PCR Primer B	1	2000128
● cDNA Primers	1	2000089

10xGenomics.com

10x  
GENOMICS

## Chromium Next GEM Single Cell Multiome Gel Bead Kit A, 16 rxns PN-1000231 (store at -80°C)

## Chromium

## Next GEM Single Cell Multiome Gel Beads A

Store at -80°C

	#	PN
Single Cell Multiome Gel Beads A	2	2000261

10xGenomics.com

10x  
GENOMICS

## Dynabeads™ MyOne™ SILANE, PN-2000048 (store at 4°C)

	#	PN
Dynabeads MyOne SILANE	2	2000048

## Chromium Next GEM Single Cell Multiome ATAC Kit A, 16 rxns PN-1000280 (store at -20°C)

Chromium Next GEM Single Cell Multiome ATAC Kit A		
Store at -20°C		
	#	PN
● 20X Nuclei Buffer	1	2000207
● ATAC Buffer B	1	2000193
● ATAC Enzyme B	1	2000265

10xGenomics.com **10x** GENOMICS

## Library Construction Kit, 16 rxns PN-1000190 (store at -20°C)

Library Construction Kit		
Store at -20°C		
	#	PN
● Fragmentation Enzyme	1	2000090
● Fragmentation Buffer	1	2000091
● Ligation Buffer	1	2000092
● DNA Ligase	1	220110
● Adaptor Oligos	1	2000094
○ Amp Mix	1	2000047

10xGenomics.com **10x** GENOMICS



## Chromium Next GEM Single Cell Multiome Reagent Kit A, 4 rxns PN-1000284

## Chromium Next GEM Single Cell Multiome GEM Kit A, 4 rxns PN-1000236 (store at -20°C)

## Chromium

## Next GEM Single Cell Multiome GEM Kit A

Store at -20°C

	#	PN
● Barcoding Reagent Mix	1	2000267
● Barcoding Enzyme Mix	1	2000273
● Template Switch Oligo	1	3000228
○ Reducing Agent B	1	2000087
● Cleanup Buffer	1	2000088
● Quenching Agent	1	2000269

10xGenomics.com

10x  
GENOMICS

## Chromium Next GEM Single Cell Multiome Amp Kit A, 4 rxns PN-1000237 (store at -20°C)

## Chromium

## Next GEM Single Cell Multiome Amp Kit A

Store at -20°C

	#	PN
● Pre-Amp Mix	1	2000274
● Pre-Amp Primers	1	2000271
○ Amp Mix	1	2000103
● SI-PCR Primer B	1	2000128
● cDNA Primers	1	2000089

10xGenomics.com

10x  
GENOMICS

## Chromium Next GEM Single Cell Multiome Gel Bead Kit A, 4 rxns PN-1000235 (store at -80°C)

## Chromium

## Next GEM Single Cell Multiome Gel Beads A

Store at -80°C

	#	PN
Single Cell Multiome Gel Beads A	1	2000261

10xGenomics.com

10x  
GENOMICS

## Dynabeads™ MyOne™ SILANE, PN-2000048 (store at 4°C)

	#	PN
Dynabeads MyOne SILANE	1	2000048

## Chromium Next GEM Single Cell Multiome ATAC Kit A, 4 rxns PN-1000281 (store at -20°C)

<b>Chromium</b>		
Next GEM Single Cell Multiome ATAC Kit A		
Store at -20°C		
	#	PN
● 20X Nuclei Buffer	1	2000207
● ATAC Buffer B	1	2000193
● ATAC Enzyme B	1	2000272

10xGenomics.com **10x** GENOMICS

## Library Construction Kit B, 4 rxns PN-1000279 (store at -20°C)

<b>Library Construction Kit B</b>		
Store at -20°C		
	#	PN
● Fragmentation Enzyme	1	2000104
● Fragmentation Buffer	1	2000091
● Ligation Buffer	1	2000092
● DNA Ligase	1	220131
● Adaptor Oligos	1	2000094
○ Amp Mix	1	2000131

10xGenomics.com **10x** GENOMICS

## Chromium Next GEM Chip J Single Cell Kit, 48 rxns PN-1000234 (store at ambient temperature)

Chromium Partitioning Oil			Chromium Recovery Agent		
	#	PN		#	PN
<input checked="" type="radio"/> Partitioning Oil	6	2000190	<input type="radio"/> Recovery Agent	6	220016

Chromium Next GEM Chip J & Gaskets		
	#	PN
Chromium Next GEM Chip J	6	2000264
Gasket, 6-pack	1	370017

10xGenomics.com 10x  
GENOMICS

## Chromium Next GEM Chip J Single Cell Kit, 16 rxns PN-1000230 (store at ambient temperature)

Chromium Partitioning Oil			Chromium Recovery Agent		
	#	PN		#	PN
<input checked="" type="radio"/> Partitioning Oil	2	2000190	<input type="radio"/> Recovery Agent	2	220016

Chromium Next GEM Chip J & Gaskets		
	#	PN
Chromium Next GEM Chip J	2	2000264
Gasket, 2-pack	1	3000072

10xGenomics.com 10x  
GENOMICS

---

### Single Index Kit N Set A, 96 rxns PN-1000212 (store at $-20^{\circ}\text{C}$ )

#### Single Index Kit N Set A

	#	PN
Single Index Plate N Set A	1	3000427

---

### Dual Index Kit TT Set A, 96 rxns PN-1000215 (store at $-20^{\circ}\text{C}$ )

#### Dual Index Kit TT Set A

	#	PN
Dual Index Plate TT Set A	1	3000431

## Chromium Accessories

Product	PN (Orderable)	PN (Item)
10x Vortex Adapter	120251	330002
Chromium Next GEM Secondary Holder	1000195	3000332
10x Magnetic Separator	120250	230003

## Recommended Thermal Cyclers

Thermal cyclers used must support uniform heating of 100  $\mu$ l emulsion volumes.

Supplier	Description	Part Number
Bio-Rad	C1000 Touch Thermal Cycler with 96-Deep Well Reaction Module	1851197
Eppendorf	MasterCycler Pro (discontinued)	North America 950030010 International 6321 000.019
Thermo Fisher Scientific	Veriti 96-Well Thermal Cycler	4375786

## Additional Kits, Reagents & Equipment

The items in the table below have been validated by 10x Genomics and are highly recommended for the Single Cell protocols. Substituting materials may adversely affect system performance. This list does not include standard laboratory equipment such as water baths, centrifuges, vortex mixers, pH meters, freezers etc.

Supplier	Description	Part Number (US)
<b>Plastics</b>		
Eppendorf	PCR Tubes 0.2 ml 8-tube strips	951010022
	DNA LoBind Tubes, 1.5 ml	022431021
	DNA LoBind Tubes, 2.0 ml	022431048
USA Scientific	TempAssure PCR 8-tube strip	1402-4700
Thermo Fisher Scientific	MicroAmp 8-Tube Strip, 0.2 ml	N8010580
	MicroAmp 8-Cap Strip, clear	N8010535
Rainin	Tips LTS 200UL Filter RT-L200FLR	30389240
	Tips LTS 1ML Filter RT-L1000FLR	30389213
	Tips LTS 20UL Filter RT-L10FLR	30389226
<b>Kits &amp; Reagents</b>		
Thermo Fisher Scientific	Nuclease-free Water	AM9937
	Low TE Buffer (10 mM Tris-HCl pH 8.0, 0.1 mM EDTA)	12090-015
Millipore Sigma	Ethanol, Pure (200 Proof, anhydrous)	E7023-500ML
	Sigma Protector RNase Inhibitor	3335399001
	DTT	646563
Beckman Coulter	SPRIselect Reagent Kit	B23318
Bio-Rad	10% Tween 20	1662404
Ricca Chemical Company	Glycerin (glycerol), 50% (v/v) Aqueous Solution	3290-32
Qiagen	Qiagen Buffer EB	19086
<b>Equipment</b>		
VWR	Vortex Mixer	10153-838
	Divided Polystyrene Reservoirs	41428-958
	VWR Mini Centrifuge	76269-066
	(alternatively, use any equivalent mini centrifuge)	
Eppendorf	Eppendorf ThermoMixer C	5382000023
	Eppendorf ThermoMixer C Bundle, includes SmartBlock 1.5 ml, Thermoblock for 24 reaction vessel (alternatively, use a temperature-controlled Heat Block)	2231000574
Rainin	Pipet-Lite Multi Pipette L8-50XLS+	17013804
	Pipet-Lite Multi Pipette L8-200XLS+	17013805
	Pipet-Lite Multi Pipette L8-10XLS+	17013802
	Pipet-Lite Multi Pipette L8-20XLS+	17013803
	Pipet-Lite LTS Pipette L-2XLS+	17014393
	Pipet-Lite LTS Pipette L-10XLS+	17014388
	Pipet-Lite LTS Pipette L-20XLS+	17014392
	Pipet-Lite LTS Pipette L-100XLS+	17014384
	Pipet-Lite LTS Pipette L-200XLS+	17014391
	Pipet-Lite LTS Pipette L-1000XLS+	17014382









## Additional Kits, Reagents & Equipment

The items in the table below have been validated by 10x Genomics and are highly recommended for the Single Cell protocols. Substituting materials may adversely affect system performance. This list does not include standard laboratory equipment such as water baths, centrifuges, vortex mixers, pH meters, freezers etc.

Supplier	Description	Part Number (US)
<b>Quantification &amp; Quality Control</b>		
Agilent	2100 Bioanalyzer Laptop Bundle High Sensitivity DNA Kit 4200 TapeStation High Sensitivity D1000 ScreenTape/Reagents High Sensitivity D5000 ScreenTape/Reagents	G2943CA 5067-4626 G2991AA 5067-5584/5067-5585 5067-5592/5067-5593
PerkinElmer	LabChip GX Touch HT Nucleic Acid Analyzer DNA High Sensitivity Reagent Kit	CLS137031 CLS760672
KAPA Biosystems	KAPA Library Quantification Kit for Illumina Platforms	KK4824

Choose Bioanalyzer,  
TapeStation,  
orLabChip based  
on availability &  
preference.

## Protocol Steps &amp; Timing

Steps	Timing	Stop & Store
<b>Nuclei Isolation</b>		
Dependent on Cell Type	~1-2 h	
<b>Step 1 – Transposition</b>		
1.1 Prepare Transposition Mix	10 min	
1.2 Isothermal Incubation	60 min	
<b>Step 2 – GEM Generation &amp; Barcoding</b>		
2.1 Prepare Master Mix	10 min	
2.2 Load Chromium Next GEM Chip J	10 min	
2.3 Run the Chromium Controller	18 min	
2.4 Transfer GEMs	3 min	
2.5 GEM Incubation	75 min	
2.6 Quenching Reaction	5 min	 -80°C ≤ 4 week
<b>Step 3 – Post GEM Incubation Cleanup</b>		
3.1 Post GEM Incubation Cleanup – Dynabeads	35 min	
3.2 Post GEM Incubation Cleanup – SPRIselect	15 min	
<b>Step 4 – Library Pre-Amplification PCR</b>		
4.1 Prepare Pre-Amplification Mix	10 min	
4.2 Pre-Amplification PCR	30 min	 4°C ≤ 18 h
4.3 SPRI Cleanup	15 min	 4°C ≤ 72 h or -20°C long-term
<b>Step 5 – Single Cell ATAC Library Construction</b>		
5.1 Sample Index PCR	45 min	
5.2 Post Sample Index Double Sided Size Selection – SPRIselect	20 min	 4°C ≤ 72 h or -20°C long-term
5.3 Post Library Construction QC	60 min	
<b>Step 6 – cDNA Amplification</b>		
6.1 cDNA Amplification	40 min	 4°C ≤ 72 h or -20°C ≤ 1 week
6.2 cDNA Cleanup – SPRIselect	15 min	 4°C ≤ 72 h or -20°C ≤ 4 weeks
6.3 cDNA QC & Quantification	50 min	
<b>Step 7 – Gene Expression Library Construction</b>		
7.1 Fragmentation, End Repair & A-tailing	45 min	
7.2 Post Fragmentation, End Repair & A-tailing Double Sided – SPRIselect	30 min	
7.3 Adaptor Ligation	25 min	
7.4 Post Ligation Cleanup- SPRIselect	20 min	
7.5 Sample Index PCR	40 min	 4°C ≤ 72 h
7.6 Post Sample Index PCR Double Sided – SPRIselect	30 min	 4°C ≤ 72 h or -20°C long term
7.7 Post Library Construction QC	50 min	



## Stepwise Objectives


Chromium Single Cell Multiome + Gene Expression provides a comprehensive, scalable multiomic approach for simultaneously profiling epigenomic landscape and gene expression in the same single nuclei. This is achieved by transposing nuclei in a bulk solution. Using a microfluidic chip, the nuclei are partitioned into nanoliter-scale Gel Beads-in-emulsion (GEMs). A pool of 736,000 10x Barcodes is sampled to separately and uniquely index the transposed DNA and cDNA of each individual nucleus. ATAC and gene expression (GEX) libraries are generated from the same pool of pre-amplified transposed DNA/cDNA and sequenced. The 10x Barcodes in each library type are used to associate individual reads back to the individual partitions, and thereby, to each individual nucleus.

### Step 1 Transposition


Nuclei suspensions are incubated in a Transposition Mix that includes a Transposase. The Transposase enters the nuclei and preferentially fragments the DNA in open regions of the chromatin. Simultaneously, adapter sequences are added to the ends of the DNA fragments.

### Step 2 GEM Generation & Barcoding

Single Cell Multiome ATAC + GEX Gel Beads include a poly(dT) sequence that enables production of barcoded, full-length cDNA from poly-adenylated mRNA for gene expression (GEX) library and a Spacer sequence that enables barcode attachment to transposed DNA fragments for ATAC library.

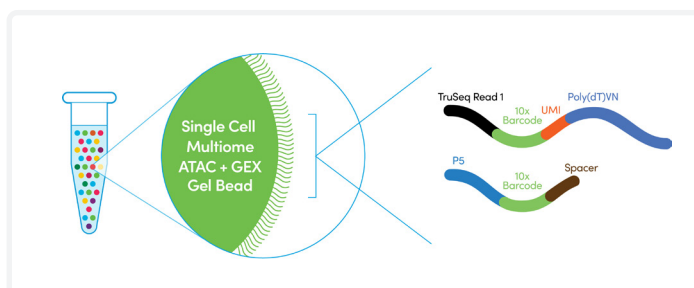


GEMs are generated by combining barcoded Gel Beads, transposed nuclei, a Master Mix, and Partitioning Oil on a Chromium Next GEM Chip J. To achieve single nuclei resolution, the nuclei are delivered at a limiting dilution, such that the majority (~90-99%) of generated GEMs contains no nuclei, while the remainder largely contain a single nucleus.

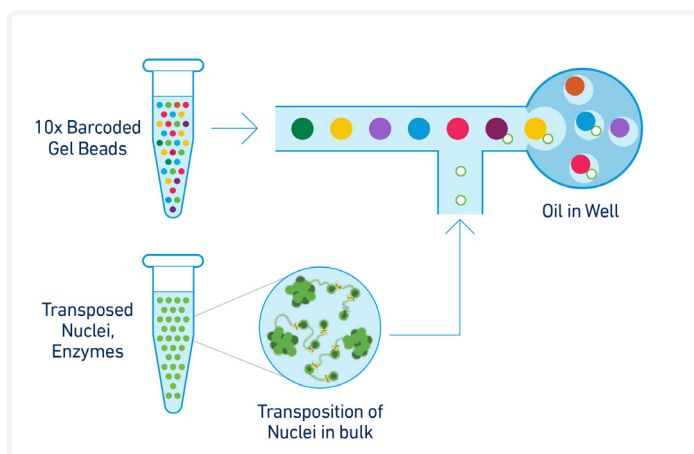

Upon GEM generation, the Gel Bead is dissolved. Oligonucleotides containing an Illumina® P5 sequence, a 16 nt 10x Barcode (for ATAC), and a Spacer sequence are released. In the same partition, primers containing an Illumina® TruSeq Read 1 (read 1 sequencing primer), 16 nt 10x Barcode (for GEX), 12 nt unique molecular identifier (UMI), and a 30 nt poly(dT) sequence are also released. The primers are mixed with the nuclei lysate containing transposed DNA fragments, mRNA, and Master Mix, that includes reverse transcription (RT) reagents.

Incubation of the GEMs produces 10x Barcoded DNA from the transposed DNA (for ATAC) and 10x Barcoded, full-length cDNA from poly-adenylated mRNA (for GEX). This is followed by a quenching step that stops the reaction.

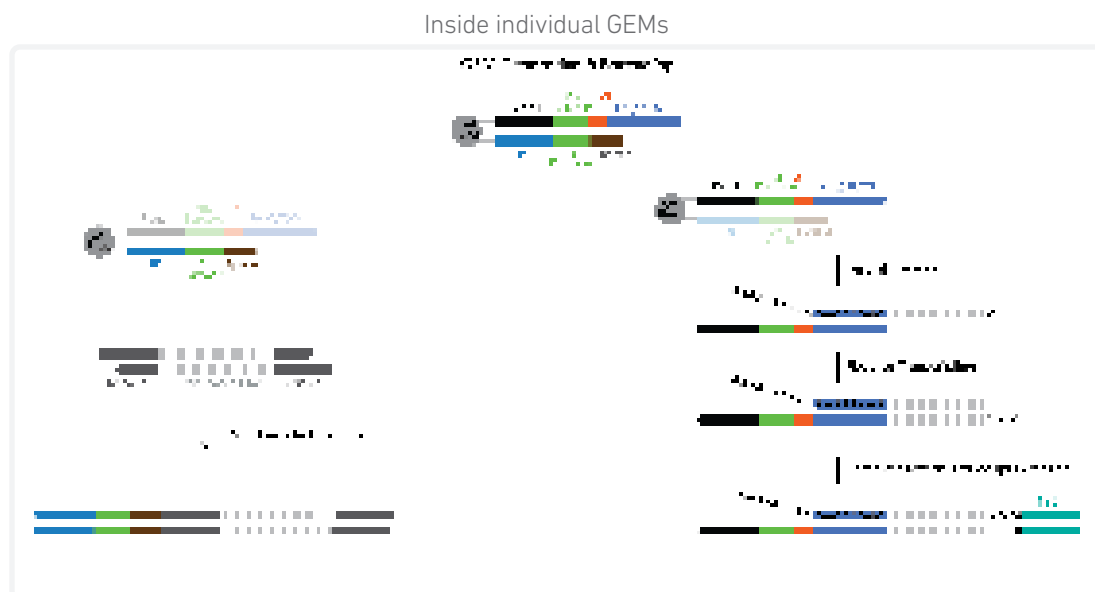


### Step 3 Post-GEM Cleanup

GEMs are broken and pooled fractions are recovered. Silane magnetic beads are used to purify the cell barcoded products from the post GEM-RT reaction mixture, which includes leftover biochemical reagents and primers.


### Step 4 Pre-Amplification PCR

Barcoded transposed DNA and barcoded full length cDNA from poly-adenylated mRNA are amplified via PCR to fill gaps and for generating sufficient mass for library construction. The pre-amplified product is used as input for both ATAC library construction and cDNA amplification for gene expression library construction.

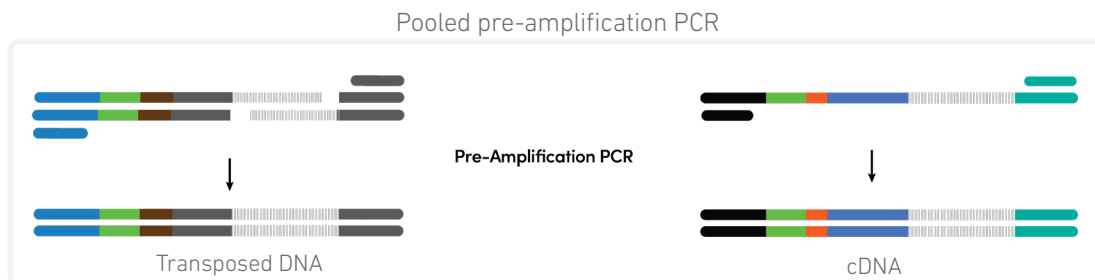

### Step 5 ATAC Library Construction

P7 and a sample index are added to pre-amplified transposed DNA during ATAC library construction via PCR. The final ATAC libraries contain the P5 and P7 sequences used in Illumina® bridge amplification.

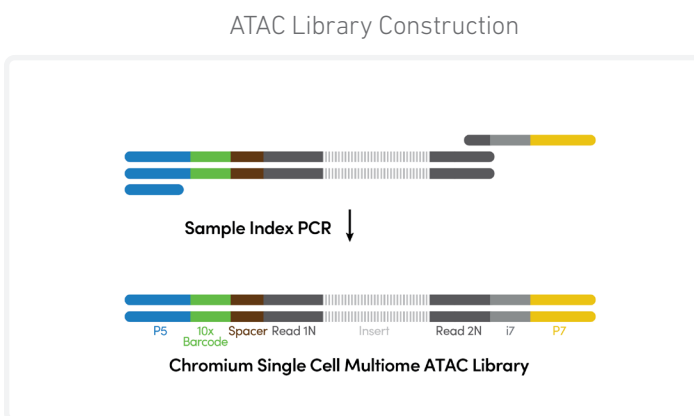


### Step 6 cDNA Amplification

Barcoded, full-length pre-amplified cDNA is amplified via PCR to generate sufficient mass for gene expression library construction.


### Step 7 Gene Expression Library Construction

Enzymatic fragmentation and size selection are used to optimize the cDNA amplicon size. P5, P7, i7 and i5 sample indexes, and TruSeq Read 2 (read 2 primer sequence) are added via End Repair, A-tailing, Adaptor Ligation, and PCR. The final gene expression libraries contain the P5 and P7 primers used in Illumina® bridge amplification.

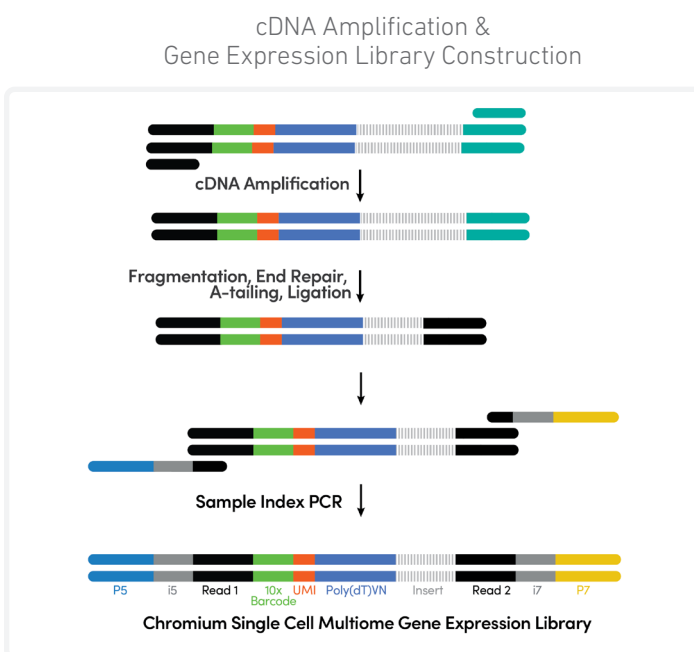


## Step 8 Sequencing

Chromium Single Cell Multiome ATAC libraries comprise double stranded DNA with standard Illumina® paired-end constructs which begin with P5 and end with P7. Sequencing these libraries produces a standard Illumina® BCL data output folder that includes paired-end Read 1N and Read 2N used for sequencing the DNA insert, along with the 8 bp sample index in the i7 read and 16 bp 10x Barcode sequence in the i5 read.

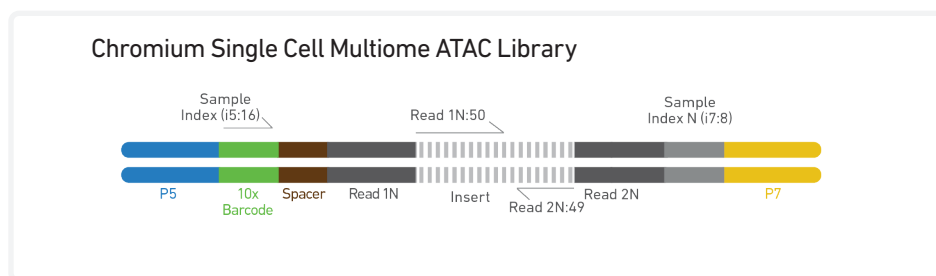

Chromium Single Cell Multiome Gene Expression libraries comprise cDNA insert with standard Illumina® paired-end constructs which begin with P5 and end with P7. Sequencing these libraries produces a standard Illumina® BCL data output folder. TruSeq Read 1 is used to sequence 16 bp 10x Barcodes and 12 bp UMI, while 10 bp i5 and i7 sample index sequences are the sample index reads. TruSeq Read 2 is used to sequence the insert.

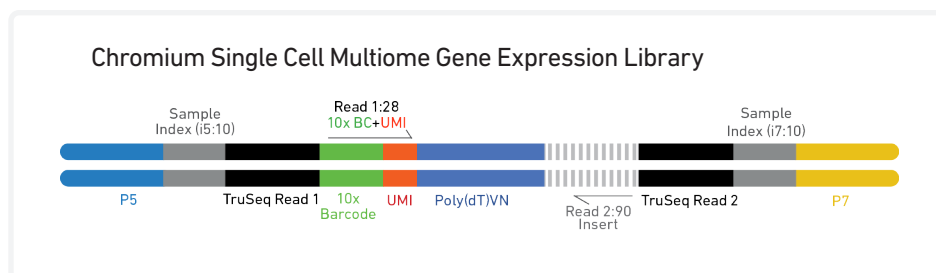

# Tips & Best Practices



Icons



Tips & Best Practices section includes additional guidance



Signifies critical step requiring accurate execution



Troubleshooting section includes additional guidance

Emulsion-safe Plastics

- Use 10x Genomics validated emulsion-safe plastic consumables when handling GEMs as some plastics can destabilize GEMs.

Multiplet Rate

Multiplet Rate (%)	# of Nuclei Loaded	# of Nuclei Recovered
0.4%	~775	~500
0.8%	~1,550	~1,000
1.6%	~3,075	~2,000
2.3%	~4,625	~3,000
3.1%	~6,150	~4,000
3.9%	~7,700	~5,000
4.6%	~9,250	~6,000
5.4%	~10,750	~7,000
6.2%	~12,300	~8,000
6.9%	~13,850	~9,000
7.7%	~15,400	~10,000

General Reagent Handling

- Fully thaw and thoroughly mix reagents before use.
- Keep all enzymes and Master Mixes on ice during setup and use. Promptly move reagents back to the recommended storage.
- Calculate reagent volumes with 10% excess of reaction volumes.
- Cover Partitioning Oil tubes and reservoirs to minimize evaporation.
- Thoroughly mix samples with the beads during bead-based cleanup steps.

---

### 50% Glycerol Solution

- Purchase 50% glycerol solution from Ricca Chemical Company, Glycerin (glycerol), 50% (v/v) Aqueous Solution, PN-3290-32.
- Prepare 50% glycerol solution:
  - i. Mix an equal volume of water and 99% Glycerol, Molecular Biology Grade.
  - ii. Filter through a 0.2  $\mu\text{m}$  filter.
  - iii. Store at  $-20^{\circ}\text{C}$  in 1-ml LoBind tubes. 50% glycerol solution should be equilibrated to room temperature before use.

---

### Pipette Calibration

- Follow manufacturer's calibration and maintenance schedules.
- Pipette accuracy is particularly important when using SPRIselect reagents.


---

### Chromium Next GEM Chip Handling

- Minimize exposure of reagents, chips, and gaskets to sources of particles and fibers, laboratory wipes, frequently opened flip-cap tubes, clothing that sheds fibers, and dusty surfaces.
- After removing the chip from the sealed bag, use in  $\leq 24$  h.
- Execute steps without pause or delay, unless indicated. When multiple chips are to be used, load, run, and collect the content from one chip before loading the next.
- Fill all unused input wells in rows labeled 1, 2, and 3 on a chip with an appropriate volume of 50% glycerol solution before loading the used wells. **DO NOT** add glycerol to the wells in the bottom NO FILL row.
- Avoid contacting the bottom surface of the chip with gloved hands and other surfaces. Frictional charging can lead to inadequate priming of the channels, potentially leading to either clogs or wetting failures.
- Minimize the distance that a loaded chip is moved to reach the Chromium Controller.
- Keep the chip horizontal to prevent wetting the gasket with oil, which depletes the input volume and may adversely affect the quality of the resulting emulsion.

### Chromium Next GEM Secondary Holders

- Chromium Next GEM Secondary Holders encase Chromium Next GEM Chips.
- The holder lid flips over to become a stand, holding the chip at 45 degrees for optimal recovery well content removal.
- Squeeze the black sliders on the back side of the holder together to unlock the lid and return the holder to a flat position.

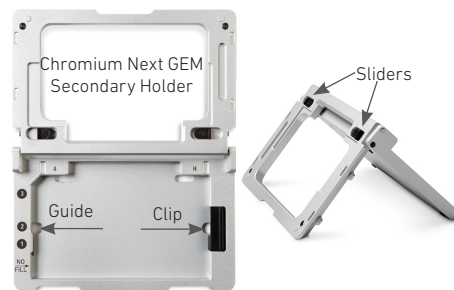

### Chromium Next GEM Chip & Holder Assembly

- Align notch on the chip (upper left corner) and the holder.
- Insert the left-hand side of the chip under the guide. Depress the right-hand side of the chip until the spring-loaded clip engages.
- Close the lid before dispensing reagents into the wells.




### Chromium Next GEM Chip Loading

- Place the assembled chip and holder flat on the bench with the lid closed.
- Dispense at the bottom of the wells without introducing bubbles.
- When dispensing Gel Beads into the chip, wait for the remainder to drain into the bottom of the pipette tips and dispense again to ensure complete transfer.
- Refer to [Load Chromium Next GEM Chip J](#) for specific instructions.



### Gel Bead Handling

- Use one tube of Gel Beads per sample. DO NOT puncture the foil seals of tubes not used at the time.
- Equilibrate the Gel Beads strip to room temperature before use.
- Store unused Gel Beads at  $-80^{\circ}\text{C}$  and avoid more than 12 freeze-thaw cycles. DO NOT store Gel Beads at  $-20^{\circ}\text{C}$ .
- Snap the tube strip holder with the Gel Bead strip into a 10x Vortex Adapter. Vortex **30 sec**.
- Centrifuge the Gel Bead strip for **~5 sec** after removing from the holder. Confirm there are no bubbles at the bottom of the tubes and the liquid levels look even. Place the Gel Bead strip back in the holder and secure the holder lid.
- If the required volume of beads cannot be recovered, place the pipette tips against the sidewalls and slowly dispense the Gel Beads back into the tubes. DO NOT introduce bubbles into the tubes and verify that the pipette tips contain no leftover Gel Beads. Withdraw the full volume of beads again by pipetting slowly.

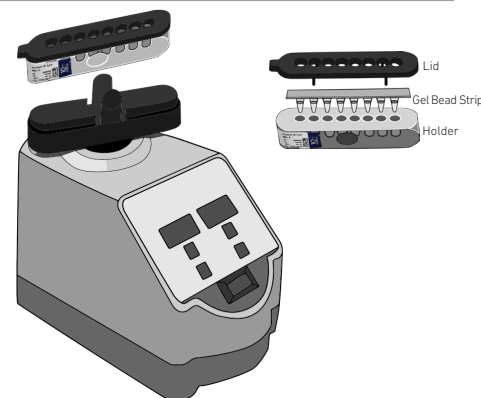




### 10x Gasket Attachment

- After reagents are loaded, attach the gasket by holding the tongue (curved end, to the right) and hook it on the left-hand tabs of the holder. Gently pull the gasket toward the right and hook it on the two right-hand tabs.
- DO NOT touch the smooth side of the gasket. DO NOT press down on the top of the gasket after attachment.
- Keep the assembly horizontal to avoid wetting the gasket with Partitioning Oil.




### 10x Magnetic Separator

- Offers two positions of the magnets (high and low) relative to a tube, depending on its orientation. Flip the magnetic separator over to switch between high (magnet•High) or low (magnet•Low) positions.
- If using MicroAmp 8-Tube Strips, use the high position (magnet•High) only throughout the protocol.

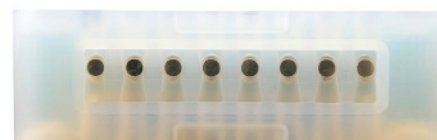

### Magnetic Bead Cleanup Steps

- During magnetic bead based cleanup steps that specify waiting “until the solution clears”, visually confirm clearing of solution before proceeding to the next step. See adjacent panel for an example.
- The time needed for the solution to clear may vary based on specific step, reagents, volume of reagents etc.

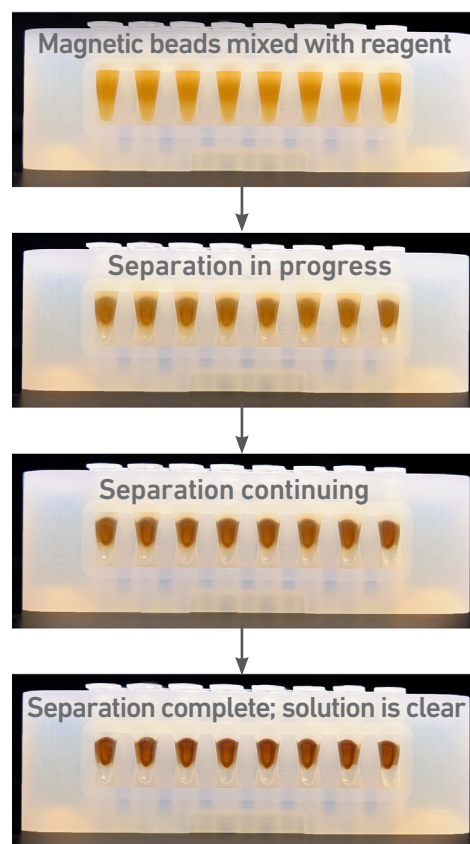

## SPRIselect Cleanup & Size Selection


- After aspirating the desired volume of SPRIselect reagent, examine the pipette tips before dispensing to ensure the correct volume is transferred.
- Pipette mix thoroughly as insufficient mixing of sample and SPRIselect reagent will lead to inconsistent results.
- Use fresh preparations of 80% Ethanol.

### Tutorial — SPRIselect Reagent:DNA Sample Ratios

SPRI beads selectively bind DNA according to the ratio of SPRIselect reagent (beads).

Example: Ratio =  $\frac{\text{Volume of SPRIselect reagent added to the sample}}{\text{Volume of DNA sample}} = \frac{50 \mu\text{l}}{100 \mu\text{l}} = 0.5X$

### Schematic of Double Sided Size Selection

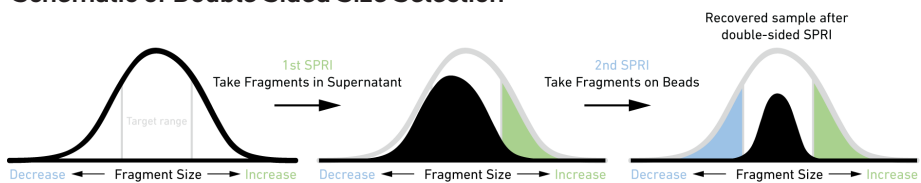

After the first SPRI, supernatant is transferred for a second SPRI while larger fragments are discarded (green). After the second SPRI, fragments on beads are eluted and kept while smaller fragments are discarded (blue). Final sample has a tight fragment size distribution with reduced overall amount (black).

### Tutorial — Double Sided Size Selection

**Step a – First SPRIselect:** Add 50  $\mu\text{l}$  SPRIselect reagent to 100  $\mu\text{l}$  sample (0.5X).

Ratio =  $\frac{\text{Volume of SPRIselect reagent added to the sample}}{\text{Volume of DNA sample}} = \frac{50 \mu\text{l}}{100 \mu\text{l}} = 0.5X$

**Step b – Second SPRIselect:** Add 30  $\mu\text{l}$  SPRIselect reagent to supernatant from step a (0.8X).

Ratio =  $\frac{\text{Total Volume of SPRIselect reagent added to the sample (step a + b)}}{\text{Original Volume of DNA sample}} = \frac{50 \mu\text{l} + 30 \mu\text{l}}{100 \mu\text{l}} = 0.8X$

## Enzymatic Fragmentation

- Ensure enzymatic fragmentation reactions are prepared on ice and then loaded into a thermal cycler pre-cooled to 4°C prior to initiating the Fragmentation, End Repair, and A-tailing incubation steps.

## Sample Indices in Sample Index PCR

- Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run.
- Each well in the Single Index plate N, Set A contains a unique mix of 4 oligos.
- Each well in the Dual Index Plate TT Set A contains a unique i7 and a unique i5 oligonucleotide.
- Verify and use the specified index plate only. DO NOT use the plates interchangeably.




# Step 1

## Transposition

- 1.1 Prepare Transposition Mix
- 1.2 Isothermal Incubation

# 1

## 1.0 Transposition

GET STARTED!					
Action		Item	10x PN	Preparation & Handling	Storage
<b>Equilibrate to Room Temperature</b>		ATAC Buffer B	2000193	Vortex, centrifuge briefly.	-20°C
		20X Nuclei Buffer* *Concentrated 20X stock; dilute 1:20 in nuclease-free water before use. (See below to Prepare Diluted Nuclei Buffer)	2000207	Thaw. Vortex, centrifuge briefly.	-20°C
<b>Place on Ice</b>		ATAC Enzyme B	2000265/ 2000272	Centrifuge briefly.	-20°C


**Nuclei\*\***  
in Diluted Nuclei Buffer  
(See below to Prepare Diluted Nuclei Buffer)



\*\*Refer to Demonstrated Protocols for Nuclei Isolation for ATAC + Gene Expression Sequencing (Documents CG000365, CG000366, CG000375). Adhering to this protocol is critical for optimal assay performance.



The use of the Tris-based Diluted Nuclei Buffer for nuclei suspension is critical for optimal assay performance. The composition of the Diluted Nuclei Buffer, including Magnesium concentration, has been optimized for the Transposition and Barcoding steps. Suspension of nuclei in a different buffer may not be compatible with the downstream protocol steps.

Prepare	Diluted Nuclei Buffer	Diluted Nuclei Buffer			
		Stock	Final	1 ml	
		Maintain at 4°C			
		20X Nuclei Buffer (PN-2000207)	20X	1X	50 µl
		DTT	1,000 mM	1 mM	1 µl
		RNase Inhibitor (confirm vendor-specific stock concentration)	40 U/µl	1 U/µl	25 µl
		Nuclease-free Water	-	-	924 µl

## Nuclei Concentration Guidelines

Based on the Targeted Nuclei Recovery, resuspend the nuclei in Diluted Nuclei Buffer to get corresponding Nuclei Stock Concentrations (see Table). This enables pipetting volumes of the Nuclei Stock for Transposition (step 1.1) to be 2-5  $\mu\text{l}$ . Higher Nuclei Stock Concentrations will result in lower pipetting volumes that may increase nuclei input variability.

Targeted Nuclei Recovery	Nuclei Stock Concentration (nuclei/ $\mu\text{l}$ )
500	160-400
1,000	320-810
2,000	650-1,610
3,000	970-2,420
4,000	1,290-3,230
5,000	1,610-4,030
6,000	1,940-4,840
7,000	2,260-5,650
8,000	2,580-6,450
9,000	2,900-7,260
10,000	3,230-8,060

### Calculate volume of Nuclei Stock and Diluted Nuclei Buffer for a total volume of 5 $\mu\text{l}$

$$\text{Volume of Nuclei Stock } (\mu\text{l}) = \frac{\text{Targeted Nuclei Recovery} \times 1.61 \text{ (Recovery efficiency factor)}}{\text{Nuclei Stock Concentration (nuclei/ } \mu\text{l)}}$$

$$\text{Volume of Diluted Nuclei Buffer* } (\mu\text{l}) = 5 \mu\text{l} - \text{volume of Nuclei Stock } (\mu\text{l})$$

\*Use ONLY Diluted Nuclei Buffer (Dilute 20X Nuclei Buffer (PN-2000207) 1:20 in nuclease-free water)

#### Example Calculation

Targeted Nuclei Recovery = 4000 nuclei

Nuclei Stock Concentration = 2500 nuclei/ $\mu\text{l}$

Recovery efficiency factor 1.61

Volume of Nuclei Stock ( $\mu\text{l}$ ) =

$$\frac{\text{Targeted Nuclei Recovery} \times 1.61 \text{ (Recovery efficiency factor)}}{\text{Nuclei Stock Concentration (nuclei/} \mu\text{l)}} = \frac{4000 \times 1.61}{2500} = 2.58 \mu\text{l}$$


$$\text{Volume of Diluted Nuclei Buffer} = 5 \mu\text{l} - 2.58 \mu\text{l} = 2.42 \mu\text{l}$$

Add calculated volumes of Diluted Nuclei Buffer and Nuclei Stock to the Transposition Mix in [step 1.1](#)

## 1.1 Prepare Transposition Mix

- a. Prepare Transposition Mix on ice. Pipette mix 10x and centrifuge briefly.

Transposition Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
● ATAC Buffer B	2000193	7.0	30.8	61.6
● ATAC Enzyme B	2000265/ 2000272	3.0	13.2	26.4
<b>Total</b>	-	<b>10.0</b>	<b>44.0</b>	<b>88.0</b>

- b. Add 10 μl Transposition Mix to a tube of a PCR 8-tube strip for each sample. Centrifuge briefly and maintain on ice.
- c. Refer to [Nuclei Concentration Guidelines](#) to calculate the volume of Nuclei Stock and Diluted Nuclei Buffer for a total volume of 5 μl.
- d. Add the calculated volume of Diluted Nuclei Buffer to the Transposition Mix. Pipette mix. Centrifuge briefly.
- e.  Gently pipette mix the Nuclei Stock. Add the calculated volume of the Nuclei Stock to the tube containing the Transposition Mix. Gently pipette mix 6x (pipette set to 10 μl). DO NOT centrifuge.

## 1.2 Isothermal Incubation

- a. Incubate in a thermal cycler using the following protocol.

Lid Temperature	Reaction Volume	Run Time hh:mm:ss
50°C	15 μl	60 min
Step	Temperature	Time
Incubate	37°C	00:60:00
Hold	4°C	Hold

- b. Immediately proceed to the next step.

# Step 2

## GEM Generation & Barcoding

- 2.1 Prepare Master Mix
- 2.2 Load Chromium Next GEM Chip J
- 2.3 Run the Chromium Controller
- 2.4 Transfer GEMs
- 2.5 GEM Incubation
- 2.6 Quenching Reaction

## 2.0 GEM Generation & Barcoding

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
<b>Equilibrate to Room Temperature</b>	Single Cell Multiome Gel Beads	2000261	Equilibrate to room temperature 30 min before loading the chip.	-80°C
	<input checked="" type="radio"/> Template Switch Oligo	3000228	Centrifuge briefly, resuspend in 80 µl Low TE Buffer. Vortex 15 sec at maximum speed, centrifuge briefly, leave at room temperature for ≥ 30 min. After resuspension, store at -80°C.	-20°C
	<input type="radio"/> Reducing Agent B	2000087	Thaw, vortex, verify no precipitate, centrifuge briefly.	-20°C
	<input checked="" type="radio"/> Barcoding Reagent Mix	2000267	Thaw, vortex, verify no precipitate, centrifuge briefly.	-20°C
<b>Place on Ice</b>	<input checked="" type="radio"/> Barcoding Enzyme Mix	2000266/ 2000273	Maintain on ice. Store at -20°C immediately after use.	-20°C
<b>Obtain</b>	<input type="radio"/> Partitioning Oil	2000190	-	Ambient
	Low TE Buffer	-	Manufacturer's recommendations.	-
	Chromium Next GEM Chip J	2000264	See Tips & Best Practices.	Ambient
	10x Gasket	370017/ 3000072	See Tips & Best Practices.	Ambient
	10x Vortex Adapter	330002	See Tips & Best Practices.	Ambient
	Chromium Next GEM Secondary Holder	3000332	See Tips & Best Practices	Ambient
	50% glycerol solution If using <8 reactions	-	See Tips & Best Practices.	-



Firmware Version 4.0 or higher is required in the Chromium Controller or the Chromium Single Cell Controller used for the protocol.



## 2.1 Prepare Master Mix

a. Prepare Master Mix on ice. Pipette mix 10x and centrifuge briefly.

Master Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
● Barcoding Reagent Mix	2000267	49.5	217.8	435.6
● Template Switch Oligo	3000228	1.1	4.8	9.7
○ Reducing Agent B	2000087	1.9	8.4	16.7
● Barcoding Enzyme Mix	2000266/ 2000273	7.5	33.0	66.0
<b>Total</b>	-	<b>60.0</b>	<b>264.0</b>	<b>528.0</b>

### Assemble Chromium Next GEM Chip J



After removing the chip from the sealed bag, use the chip in  $\leq 24$  h.



See Tips & Best Practices for chip handling instructions.

- Align notch on the chip (upper left corner) and the holder.
- Insert the left-hand side of the chip under the guide. Depress the right-hand side of the chip until the spring-loaded clip engages.
- Close the lid before dispensing reagents into the wells.
- The assembled chip is ready for loading the indicated reagents. Refer to step 2.2 for reagent volumes and loading order.



For GEM generation, load the indicated reagents only in the specified rows, starting from row labeled 1, followed by rows labeled 2 and 3. DO NOT load reagents in the bottom row labeled NO FILL. See step 2.2 for details.



2.2  
Load Chromium  
Next GEM Chip J

**a. Dispense 50% Glycerol into Unused Chip Wells** (if < 8 samples per chip)

- i. 70  $\mu$ l to unused wells in row labeled 1.
  - ii. 50  $\mu$ l to unused wells in row labeled 2.
  - iii. 45  $\mu$ l to unused wells in row labeled 3.
- DO NOT add 50% glycerol solution to the bottom row of NO FILL wells. DO NOT use any substitute for 50% glycerol solution.

**b. Prepare Master Mix + Transposed Nuclei**

Add 60  $\mu$ l Master Mix to each tube containing Transposed Nuclei for a total of 75  $\mu$ l in each tube.

**c. Load Row Labeled 1**


Gently pipette mix the Master Mix + Transposed Nuclei 5x. Using the same pipette tip, dispense 70  $\mu$ l Master Mix + Transposed Nuclei into the bottom center of each well in row labeled 1 without introducing bubbles.

**!** After removing the chip from the sealed bag, use in  $\leq$  24 h. For all chip loading steps, raising and depressing the pipette plunger should each take  $\sim$ 5 sec. When dispensing, raise the pipette tips at the same rate as the liquid is rising, keeping the tips slightly submerged.



**d. Prepare Gel Beads**

Snap the tube strip holder with the Gel Bead strip into a 10x Vortex Adapter. Vortex 30 sec. Centrifuge the Gel Bead strip for  $\sim$ 5 sec. Confirm there are no bubbles at the bottom of the tubes and the liquid levels are even. Place the Gel Bead strip back in the holder. Secure the holder lid.

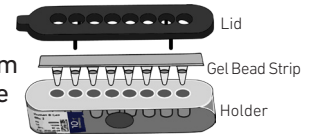

**e. Load Row Labeled 2**

Puncture the foil seal of the Gel Bead tubes. Slowly aspirate 50  $\mu$ l Gel Beads. Dispense into the wells in row labeled 2 without introducing bubbles. Wait 30 sec.



**f. Load Row Labeled 3**

Dispense 45  $\mu$ l Partitioning Oil into the wells in row labeled 3 from a reagent reservoir. Failure to add Partitioning Oil to the top row labeled 3 will prevent GEM generation and can damage the Chromium Controller.



**!** Attach the gasket and run the chip in the Chromium Controller immediately after loading the Partitioning Oil.

**g. Attach 10x Gasket**

Align the notch with the top left-hand corner. Ensure the gasket holes are aligned with the wells. Avoid touching the smooth surface.



### 2.3 Run the Chromium Controller

- Press the eject button on the Controller to eject the tray.
- Place the assembled chip with the gasket in the tray, ensuring that the chip stays horizontal. Press the button to retract the tray.
- Confirm the program on screen "Chromium Chip J". Press the play button.
- At completion of the run (~18 min), the Controller will chime. **Immediately** proceed to the next step.



Firmware Version 4.00 or higher is required in the Chromium Controller or the Chromium Single Cell Controller used for the protocol.



### 2.4 Transfer GEMs

- Place a PCR 8-tube strip on ice.
- Press the eject button of the Controller to remove the chip.
- Discard the gasket. Open the chip holder. Fold the lid back until it clicks to expose the wells at 45 degrees.
- Check the volume in row labeled 1-2. Abnormally high volume in any well indicates a clog.
- Slowly aspirate 100  $\mu$ l GEMs from the lowest points of the recovery wells in the top row labeled 3 without creating a seal between the pipette tips and the wells.
- Withdraw pipette tips from the wells. GEMs should appear opaque and uniform across all channels. Excess Partitioning Oil (clear) in the pipette tips indicates a potential clog.
- Over the course of ~20 sec, dispense GEMs into the tube strip on ice with the pipette tips against the sidewalls of the wells.
- If multiple chips are run back-to-back, cap/cover the GEM-containing tube strip or plate and place on ice for no more than 1 h.



#### Expose Wells at 45 Degrees



#### Transfer GEMs



#### GEMs



## 2.5 GEM Incubation

Use a thermal cycler that can accommodate at least 100  $\mu\text{l}$  volume. A volume of 125  $\mu\text{l}$  is the preferred setting on Bio-Rad C1000 Touch. In alternate thermal cyclers, use highest reaction volume setting.

Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time hh:mm:ss
50°C	100 $\mu\text{l}$	75 min
Step	Temperature	Time
1	37°C	00:45:00
2	25°C	00:30:00
3	4°C	Hold (not overnight*)



Retrieve Quenching Agent (● PN-2000269) from -20°C and equilibrate to **room temperature** while the PCR program is running.

\*After GEM incubation, proceed **immediately** to the next step.

## 2.6 Quenching Reaction



- Add 5  $\mu\text{l}$  Quenching Agent to each sample to stop the reaction.
- Slowly pipette mix 10x (pipette set to 90  $\mu\text{l}$ ). The solution will be viscous. Ensure that no liquid remains along the tube sidewalls and pipette tips. If necessary, aspirate the entire volume and dispense back slowly into the tube.



- Store at -80°C for up to 4 weeks, or proceed to the next step.

# Step 3

## Post GEM Incubation Cleanup

- 3.1 Post GEM Incubation Cleanup – Dynabeads
- 3.2 Post GEM Incubation Cleanup – SPRIselect



### 3.0 Post GEM Incubation Cleanup

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
<b>Equilibrate to Room Temperature</b>	<input type="radio"/> Reducing Agent B	2000087	Thaw, vortex, verify no precipitate, centrifuge briefly.	-20°C
	Nuclease-free Water	-	-	-
	Dynabeads MyOne SILANE	2000048	Vortex thoroughly ( $\geq 30$ sec) to resuspend beads immediately before use.	4°C
	Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
<b>Thaw at 65°C</b>	<input type="radio"/> Cleanup Buffer	2000088	Thaw for 10 min at 65°C at max speed on a thermomixer. Verify there are no visible crystals. Cool to room temperature.	-20°C
<b>Obtain</b>	Recovery Agent	220016	-	Ambient
	Qiagen Buffer EB	-	Manufacturer's recommendations.	-
	Bio-Rad 10% Tween 20	-	Manufacturer's recommendations.	-
	10x Magnetic Separator	230003	-	Ambient
	Prepare 80% Ethanol Prepare 10 ml for 8 reactions	-	Prepare fresh.	-

### 3.1 Post GEM Incubation Cleanup – Dynabeads

- a. Add **125  $\mu$ l** Recovery Agent to each sample at room temperature. **DO NOT** pipette mix or vortex the biphasic mixture. Gently invert tube 10x to mix. Centrifuge briefly.

The resulting biphasic mixture contains Recovery Agent/Partitioning Oil (pink) and aqueous phase (clear), with no persisting emulsion (opaque).





A smaller aqueous phase volume indicates a clog during GEM generation.



- b. Slowly remove and discard **125  $\mu$ l** Recovery Agent/Partitioning Oil (pink) from the bottom of the tube. **DO NOT** aspirate any aqueous sample.



- c. Prepare Dynabeads Cleanup Mix.

Dynabeads Cleanup Mix <i>Add reagents in the order listed</i>	PN	1X ( $\mu$ l)	4X + 10% ( $\mu$ l)	8X + 10% ( $\mu$ l)
● Cleanup Buffer	2000088	182.0	801.0	1,602.0
Dynabeads MyOne SILANE Vortex thoroughly ( $\geq 30$ sec) <b>immediately</b> before adding to the mix.				
  Aspirate the full liquid volume with a pipette tip to verify that the beads have not settled in the bottom of the tube. If clumps are present, pipette mix to resuspend completely. <b>DO NOT</b> centrifuge before use.	2000048	13.0	57.2	114.4
○ Reducing Agent B	2000087	5.0	22.0	44.0
<b>Total</b>	-	<b>200.0</b>	<b>880.2</b>	<b>1760.4</b>



Resuspend clump



- d. Vortex and add **200  $\mu$ l** Dynabeads Cleanup Mix to each sample. Pipette mix 10x (pipette set to 200  $\mu$ l).
- e. Incubate **10 min** at room temperature (keep caps open).

#### Add Dynabeads Cleanup Mix



## f. Prepare Elution Solution I. Vortex and centrifuge briefly.

Elution Solution I* <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 15% (μl)	8X + 15% (μl)
Buffer EB	-	49.0	225.4	450.8
10% Tween 20	-	0.5	2.3	4.6
<input type="radio"/> Reducing Agent B	200087	0.5	2.3	4.6
<b>Total</b>	-	<b>50</b>	<b>230</b>	<b>460</b>



- g. At the end of **10 min** incubation, place on the 10x Magnetic Separator, high position (magnet•**High**) until the solution clears.
- h. Remove the supernatant.
- i. Add **300 μl** freshly prepared 80% ethanol to the pellet while on the magnet•**High**. Wait **30 sec**.
- j. Remove the ethanol.
- k. Add **200 μl** 80% ethanol to pellet. Wait **30 sec**.
- l. Remove the ethanol.
- m. Centrifuge briefly. Place on the magnet•**Low**.
- n. Remove remaining ethanol.
- o. Remove from the magnet. **Immediately** add **50 μl** Elution Solution I to avoid clumping.
- p. Pipette mix (pipette set to 50 μl) without introducing bubbles.
- q. Incubate **1 min** at **room temperature**.
- r. Centrifuge briefly. Place on the magnet•**Low** until the solution clears.
- s. Transfer **50 μl** sample to a new tube strip.



### 3.2 Post GEM Incubation Cleanup – SPRIselect

- a. Vortex the SPRIselect reagent until fully resuspended. Add **90  $\mu$ l** SPRIselect reagent to each sample. Pipette mix thoroughly.
- b. Incubate **5 min** at **room temperature**.
- c. Centrifuge briefly. Place on the magnet•**High** until the solution clears.
- d. Remove the supernatant.
- e. Add **200  $\mu$ l** 80% ethanol to the pellet. Wait **30 sec**.
- f. Remove the ethanol.
- g. **Repeat** steps e and f for a total of 2 washes.
- h. Centrifuge briefly. Place on the magnet•**Low**.
- i. Remove any remaining ethanol.  
Residual ethanol can inhibit Pre-Amplification PCR and impact assay performance.
- j. Remove the tube strip from the magnet. **Immediately** add **46.5  $\mu$ l** Buffer EB.
- k. Pipette mix (pipette set to 45  $\mu$ l) without introducing bubbles.
- l. Incubate **2 min** at **room temperature**.
- m. Centrifuge briefly. Place on the magnet•**Low** until the solution clears.



- n. Transfer **46  $\mu$ l** sample to a new tube strip.  
Residual SPRI beads can inhibit Pre-Amplification PCR and impact assay performance.

# Step 4

## Pre-Amplification PCR

- 4.1 Prepare Pre-Amplification Mix
- 4.2 Pre-Amplification PCR
- 4.3 SPRI Cleanup



## 4.0 Pre-Amplification PCR

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
<b>Equilibrate to Room Temperature</b>	● Pre-Amp Primers	2000271	Vortex, centrifuge briefly.	-20°C
	Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
<b>Place on Ice</b>	● Pre-Amp Mix	2000270/ 2000274	Gently pipette mix, centrifuge briefly.	-20°C
<b>Obtain</b>	Qiagen Buffer EB	-	-	Ambient
	10x Magnetic Separator	230003	See Tips & Best Practices.	Ambient
	<b>Prepare 80% Ethanol</b> Prepare 10 ml for 8 reactions	-	Prepare fresh.	Ambient

#### 4.1 Prepare Pre- Amplification Mix

a. Prepare Pre-Amplification Mix on ice. Pipette mix 10x and centrifuge briefly.

Master Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
● Pre-Amp Mix	2000270/ 2000274	50.0	220.0	440.0
● Pre-Amp Primers	2000271	4.0	17.6	35.2
<b>Total</b>	-	<b>54.0</b>	<b>237.6</b>	<b>475.2</b>

b. Add 54 μl Pre-Amplification Mix to each sample. Pipette mix and centrifuge briefly.

#### 4.2 Pre-Amplification PCR

a. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time hh:mm:ss
105°C	100 μl	30 min
Step	Temperature	Time
1	72°C	00:05:00
2	98°C	00:03:00
3	98°C	00:00:20
4	63°C	00:00:30
5	72°C	00:01:00 Go to step 3 repeat 6X (Total 7 cycles)
6	72°C	00:01:00
7	4°C	Hold



b. Store at 4°C for up to 18 h or proceed to the next step.

### 4.3 Pre-Amplification SPRI Cleanup


- a. Vortex the SPRIselect reagent until fully resuspended. Add **160  $\mu$ l** SPRIselect reagent to each sample. Pipette mix thoroughly.
- b. Incubate **5 min** at **room temperature**.
- c. Centrifuge briefly. Place on the magnet•**High** until the solution clears.
- d. Remove the supernatant.
- e. Add **300  $\mu$ l** 80% ethanol to the pellet. Wait **30 sec**.
- f. Remove the ethanol.
- g. Add **200  $\mu$ l** 80% ethanol to the pellet. Wait **30 sec**.
- h. Remove the ethanol.
- i. Centrifuge briefly. Place on the magnet•**Low**.
- j. Remove any remaining ethanol.
- k. Remove the tube strip from the magnet. **Immediately** add **160.5  $\mu$ l** Buffer EB.
- l. Pipette mix (pipette set to 150  $\mu$ l) without introducing bubbles.
- m. Incubate **2 min** at **room temperature**.
- n. Centrifuge briefly. Place on the magnet•**High** until the solution clears.
- o. Transfer **160  $\mu$ l** sample to a new tube strip.
- p. Store at **4°C** for up to **72 h** or at **-20°C** for long term storage, or proceed to the next step.



## Sample Split Overview

- **160  $\mu$ l pre-amplified, SPRI cleaned sample** derived at step 4.3p includes barcoded transposed DNA fragments and barcoded cDNA.
- The sample is divided and used as input for two separate steps.
  - I. 40  $\mu$ l sample is used for ATAC Library Construction (step 5)
  - II. 35  $\mu$ l sample is used for cDNA Amplification (step 6).  
The amplified cDNA will be used for Gene Expression Library Construction.

Store the remaining pre-amplification product at  $-20^{\circ}\text{C}$  long term for generating additional libraries.

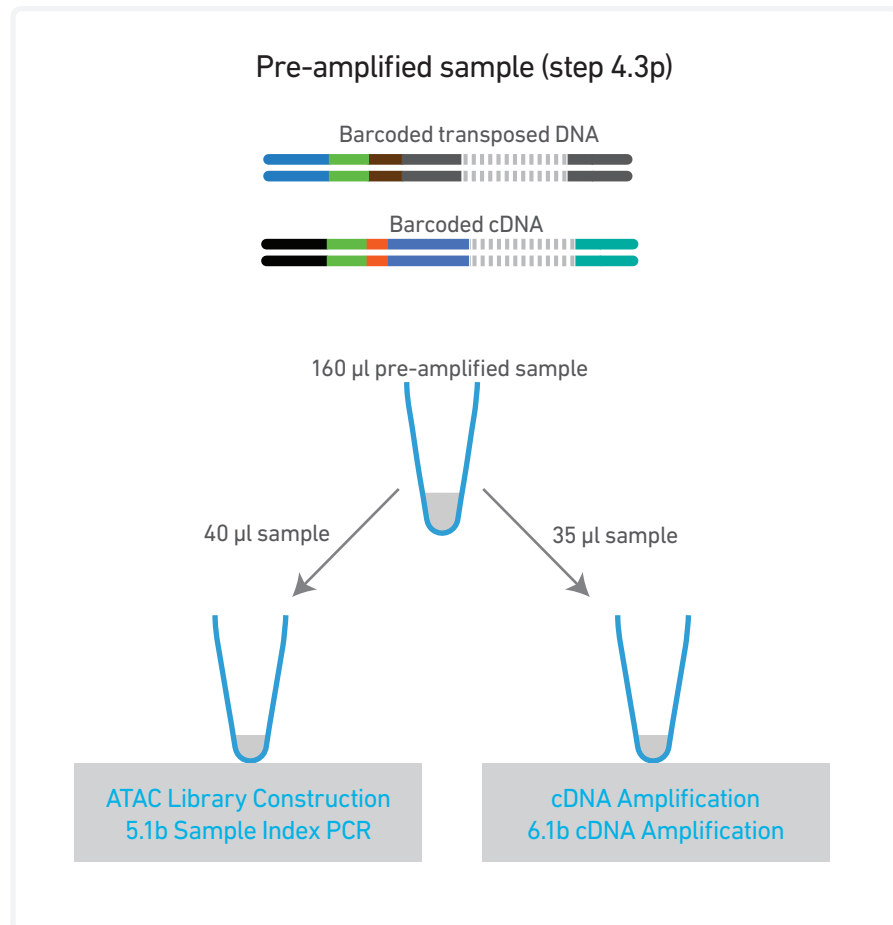

# Step 5

## ATAC Library Construction

- 5.1 Sample Index PCR
- 5.2 Post Sample Index Double Sided Size Selection – SPRIselect
- 5.3 Post Library Construction QC



## 5.0 ATAC Library Construction

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
<b>Equilibrate to Room Temperature</b>	<b>Sample Index Plate N, Set A</b>	3000427	-	-20°C
	<b>Beckman Coulter SPRiselect Reagent</b>	-	Manufacturer's recommendations.	-
	<b>Agilent Bioanalyzer DNA kit</b> If used for QC	-	Manufacturer's recommendations.	-
	<b>DNA High Sensitivity Reagent Kit</b> If LabChip used for QC	-	Manufacturer's recommendations.	-
<b>Place on Ice</b>	<input checked="" type="radio"/> <b>SI-PCR Primer B</b>	2000128	Vortex, centrifuge briefly.	-20°C
	<input type="radio"/> <b>Amp Mix</b>	2000047/ 2000103	Gently pipette mix, centrifuge briefly.	-20°C
	<b>KAPA Library Quantification Kit for Illumina® Platforms</b>	-	Manufacturer's recommendations.	-
<b>Obtain</b>	<b>Qiagen Buffer EB</b>	-	-	Ambient
	<b>10x Magnetic Separator</b>	230003	See Tips & Best Practices.	Ambient
	<b>Prepare 80% Ethanol</b> Prepare 10 ml for 8 reactions	-	Prepare fresh.	Ambient



## 5.1 Sample Index PCR

Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run.

### a. Prepare Sample Index PCR Mix.

Sample Index PCR Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
<input type="radio"/> Amp Mix	2000047/ 2000103	50	220	440
<input checked="" type="radio"/> SI- PCR Primer B	2000128	7.5	33	66
<b>Total</b>	-	<b>57.5</b>	<b>253</b>	<b>506</b>

b. Transfer **40 μl** pre-amplified sample from step 4.3p to a new tube strip (**35 μl** of the remaining sample volume will be used for cDNA Amplification and the rest can be stored at **-20°C** long term for generating additional libraries). Add **57.5 μl** Sample Index PCR Mix to the sample. Pipette mix and centrifuge briefly.

c. Add **2.5 μl** of an individual Sample Index N, Set A to each well. Record assignment. Pipette mix and centrifuge briefly.

d. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time hh:mm:ss
105°C	100 μl	~30 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	67°C	00:00:30
4	72°C	00:00:20 Go to step 2, see table below for # cycles
5	72°C	00:01:00
6	4°C	Hold

The table recommends a starting point for cycle number optimization for based on Targeted Nuclei Recovery.

Cycle Number Optimization Table

Targeted Nuclei Recovery	Total Cycles
≤2,000	9
2,001-6,000	8
6,001-10,000	7



e. Store at **4°C** for up to **72 h** or proceed to the next step.

5.2  
Post Sample Index  
Double Sided Size  
Selection – SPRIselect




- a. Vortex to resuspend SPRIselect reagent. Add **60 µl** SPRIselect reagent (0.6X) to each sample. Pipette mix.
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears.
- d. Transfer **150 µl** supernatant to a new strip tube. **DO NOT** discard the supernatant.
- e. Vortex to resuspend SPRIselect reagent. Add **95 µl** SPRIselect reagent (1.55X) to each sample (supernatant). Pipette mix.
- f. Incubate **5 min** at **room temperature**.
- g. Place on the magnet•**High** until the solution clears.
- h. Remove the supernatant.
- i. Add **300 µl** 80% ethanol to the pellet. Wait **30 sec**.
- j. Remove the ethanol.
- k. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- l. Remove the ethanol.
- m. Centrifuge briefly. Place on the magnet•**Low**.
- n. Remove remaining ethanol.
- o. Remove from the magnet. **Immediately** add **20.5 µl** Buffer EB. Pipette mix.
- p. Incubate **2 min** at **room temperature**.
- q. Centrifuge briefly. Place on the magnet•**Low** until the solution clears.
- r. Transfer **20 µl** sample to a new tube strip.
- s. Store at **4°C** for up to **72 h** or at **-20°C** for **long-term** storage.



## 5.3

Post Library Construction  
QC

- a. Run 1  $\mu\text{L}$  sample on the Agilent Bioanalyzer High Sensitivity DNA chip to determine fragment size. Select the region between 150-1000 bp to determine average size of ATAC library. Lower molecular weight product ( $\leq 150$  bp) and/or a high molecular weight product ( $\sim 2,000$  bp) may be present. This does not affect sequencing.

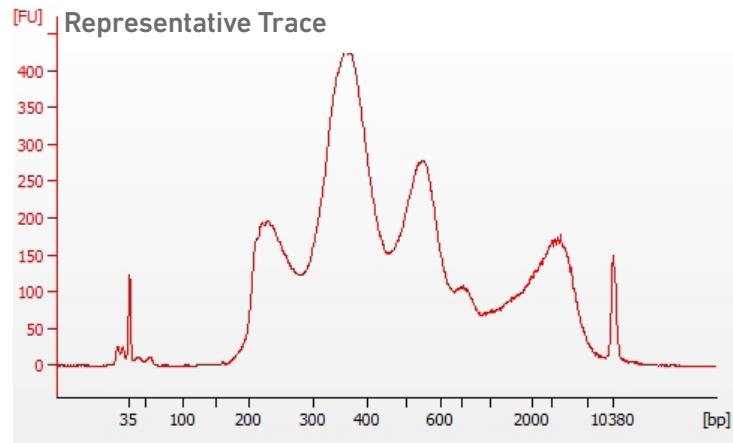**Alternate QC Methods** ([See Appendix for representative traces](#))

- Agilent TapeStation
- LabChip

[See Appendix for Post Library Construction Quantification](#)

# Step 6

## cDNA Amplification

- 6.1 cDNA Amplification
- 6.2 cDNA Cleanup – SPRIselect
- 6.3 cDNA QC & Quantification

## 6.0 cDNA Amplification

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
<b>Equilibrate to Room Temperature</b>	● <b>cDNA Primers</b>	2000089	Vortex, centrifuge briefly.	-20°C
	<b>Beckman Coulter SPRIselect Reagent</b>	-	Manufacturer's recommendations.	-
	<b>Agilent Bioanalyzer High Sensitivity Kit</b> If used for QC and quantification	-	Manufacturer's recommendations.	-
	<b>Agilent TapeStation ScreenTape and Reagents</b> If used for QC and quantification	-	Manufacturer's recommendations.	-
	<b>Qubit dsDNA HS Assay Kit</b> If used for QC and quantification	-	Manufacturer's recommendations.	-
<b>Place on ice</b>	○ <b>Amp Mix</b>	2000047/ 2000103	Vortex, centrifuge briefly.	-20°C
<b>Obtain</b>	<b>Qiagen Buffer EB</b>	-	Manufacturer's recommendations.	-
	<b>10x Magnetic Separator</b>	230003	-	Ambient
	<b>Prepare 80% Ethanol</b> Prepare 15 ml for 8 reactions.	-	-	-

## 6.1 cDNA Amplification

a. Prepare cDNA Amplification Mix on ice. Vortex and centrifuge briefly.

cDNA Amplification Reaction Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
○ Amp Mix	2000047/ 2000103	50	220	440
● cDNA Primers	2000089	15	66	132
<b>Total</b>	-	<b>65</b>	<b>286</b>	<b>572</b>

b. Transfer **35 μl** pre-amplified sample from step 4.3p to a new tube strip (store the remaining pre-amplification product at **-20°C** long term for generating additional libraries). Add **65 μl** cDNA Amplification Reaction Mix to the sample.

c. Pipette mix 15x (pipette set to 90 μl). Centrifuge briefly.

d. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~30-45 min
Step	Temperature	Time
1	98°C	00:03:00
2	98°C	00:00:15
3	63°C	00:00:20
4	72°C	00:01:00
5	Go to Step 2, see table below for total # of cycles	
6	72°C	00:01:00
7	4°C	Hold

The optimal number of cycles is a trade-off between generating sufficient final mass for library construction and minimizing PCR amplification artifacts. The number of cDNA cycles should also be reduced if large numbers of nuclei are sampled.

Recommended starting point for cycle number optimization.

Targeted Nuclei Recovery	Total Cycles
≤2,000	9
2,001–6,000	7
≥6,001	6



e. Store at **4°C** for up to **72 h** or **-20°C** for **≤1 week**, or proceed to the next step.


## 6.2 cDNA Cleanup – SPRIselect

- a. Vortex to resuspend the SPRIselect reagent. Add **60 µl** SPRIselect reagent (**0.6X**) to each sample and pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears.
- d. Remove the supernatant.
- e. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- f. Remove the ethanol.
- g. **Repeat** steps e and f for a total of 2 washes.
- h. Centrifuge briefly and place on the magnet•**Low**.
- i. Remove any remaining ethanol. Air dry for **2 min**. **DO NOT** exceed **2 min** as this will decrease elution efficiency.
- j. Remove from the magnet. Add **40.5 µl** Buffer EB. Pipette mix 15x.
- k. Incubate **2 min** at **room temperature**.
- l. Place the tube strip on the magnet•**High** until the solution clears.
- m. Transfer **40 µl** sample to a new tube strip.
- n. Store at **4°C** for up to **72 h** or at **-20°C** for up to **4 weeks**, or proceed to the next step.



### 6.3 cDNA QC & Quantification


- a. Run 1  $\mu\text{l}$  undiluted sample on an Agilent Bioanalyzer High Sensitivity chip. For input cells with low RNA content ( $<1$  pg total RNA/cell), 1  $\mu\text{l}$  undiluted product may be run. Lower molecular weight product (35 – 150 bp) may be present. This is normal and does not affect sequencing or application performance.

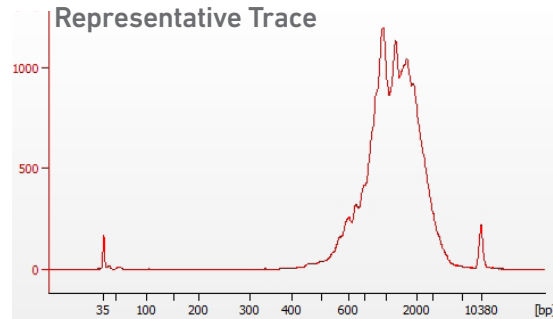


#### EXAMPLE CALCULATION

##### i. Select Region

Under the “Electropherogram” view choose the “Region Table”. Manually select the region of ~200 – ~9000 bp

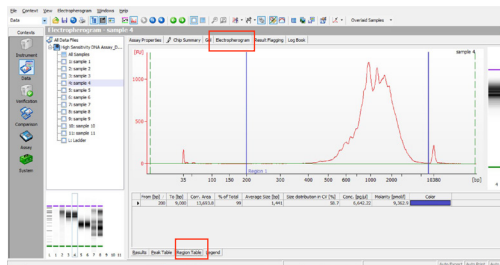

##### ii. Note Concentration [pg/ $\mu\text{l}$ ]

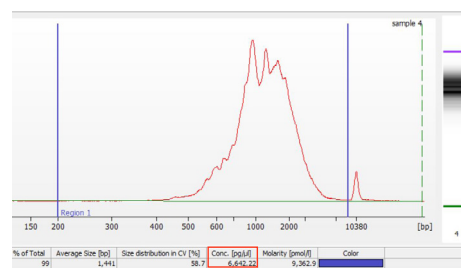

##### iii. Calculate

Multiply the cDNA concentration [pg/ $\mu\text{l}$ ] reported via the Agilent 2100 Expert Software by the elution volume (40  $\mu\text{l}$ ) of the Post cDNA Amplification Reaction Clean Up sample (taking any dilution factors into account) and then divide by 1000 to obtain the total cDNA yield in ng.

##### Example Calculation of cDNA Total Yield

Concentration: 6642.22 pg/ $\mu\text{l}$

Elution Volume: 40

Dilution Factor: 1

Total cDNA Yield

$$= \frac{\text{Conc'n (pg}/\mu\text{l}) \times \text{Elution Volume } (\mu\text{l}) \times \text{Dilution Factor}}{1000 \text{ (pg/ng)}}$$

$$= \frac{6642.22 \text{ (pg}/\mu\text{l}) \times 40 \text{ } (\mu\text{l}) \times 1}{1000 \text{ (pg/ng)}}$$

**!** Carry forward **ONLY 25%** of total cDNA yield into 3' Gene Expression Library Construction (step 3)

$$= 0.25 \times \text{Total cDNA yield}$$

$$= 0.25 \times 265.69 = 66.42 \text{ ng}$$

Refer to step 7.5 for appropriate number of Sample Index PCR cycles based on carry forward cDNA yield/input cDNA.

#### Alternate Quantification Methods (See Appendix for representative traces)

- Agilent TapeStation
- LabChip

Agilent Bioanalyzer, Agilent TapeStation, or LabChip are the recommended methods for accurate quantification.



# Step 7

## Gene Expression Library Construction

- 7.1** Fragmentation, End Repair & A-tailing
- 7.2** Post Fragmentation End Repair & A-tailing Double Sided Size Selection – SPRIselect
- 7.3** Adaptor Ligation
- 7.4** Post Ligation Cleanup – SPRIselect
- 7.5** Sample Index PCR
- 7.6** Post Sample Index PCR Double Sided Size Selection – SPRIselect
- 7.7** Post Library Construction QC


## 7.0 Gene Expression Library Construction

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
<b>Equilibrate to Room Temperature</b>	● Fragmentation Buffer	2000091	Vortex, verify no precipitate, centrifuge briefly.	-20°C
	● Adaptor Oligos	2000094	Vortex, centrifuge briefly.	-20°C
	● Ligation Buffer	2000092	Vortex, verify no precipitate, centrifuge briefly.	-20°C
	Dual Index Plate TT Set A	3000431	-	-20°C
	Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
	Agilent TapeStation Screen Tape and Reagents If used for QC		Manufacturer's recommendations.	
	Agilent Bioanalyzer High Sensitivity kit If used for QC	-	Manufacturer's recommendations.	-
	DNA High Sensitivity Reagent Kit If LabChip used for QC	-	Manufacturer's recommendations.	-
<b>Place on Ice</b>	● Fragmentation Enzyme	2000090/ 2000104	Centrifuge briefly.	-20°C
	● DNA Ligase	220110/ 220131	Centrifuge briefly.	-20°C
	○ Amp Mix	2000047/ 2000131	Centrifuge briefly.	-20°C
	KAPA Library Quantification Kit for Illumina Platforms	-	Manufacturer's recommendations.	-
<b>Obtain</b>	Qiagen Buffer EB	-	-	Ambient
	10x Magnetic Separator	230003	See Tips & Best Practices.	Ambient
	Prepare 80% Ethanol Prepare 20 ml for 8 reactions	-	Prepare fresh.	Ambient





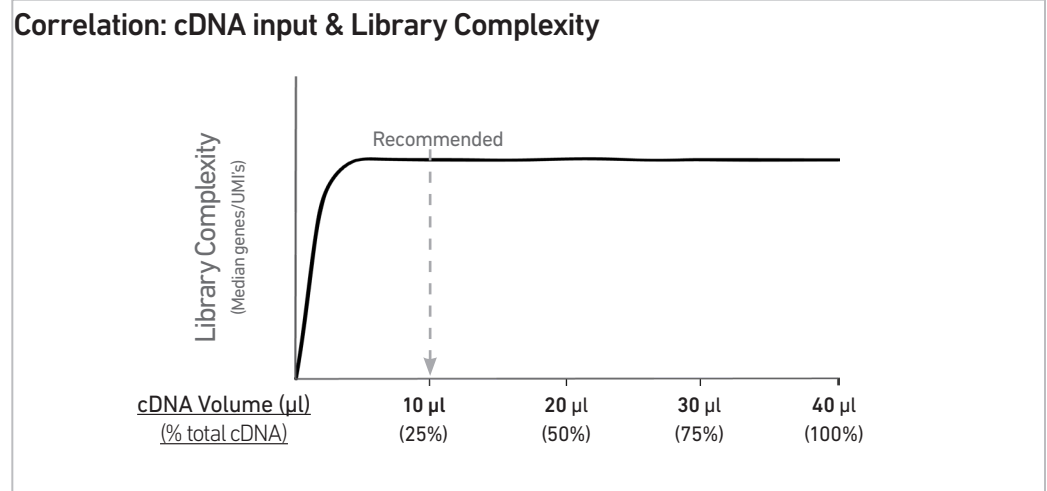

## Step Overview (Step 7.1d)

### Correlation between input & library complexity

A Single Cell Gene Expression library is generated using a fixed proportion (10  $\mu\text{l}$ , 25%) of the total cDNA (40  $\mu\text{l}$ ) obtained at step 6.2n. The complexity of this library will be comparable to one generated using a higher proportion (>25%) of the cDNA. The remaining proportion (30  $\mu\text{l}$ , 75%) of the cDNA may be stored at 4°C for up to 72 h or at -20°C for longer-term storage (up to 4 weeks).



Note that irrespective of the total cDNA yield (ng), which may vary based on cell type, targeted nuclei recovery etc., this protocol has been optimized for a broad range of input mass (ng), as shown in the example below. The total number of SI PCR cycles (step 7.5d) should be optimized based on carrying forward a fixed proportion (10  $\mu\text{l}$ , 25%) of the total cDNA yield calculated during Post cDNA Amplification QC & Quantification (step 6.3).

Example: Library Construction Input Mass & SI PCR Cycles					
Cell Type	Targeted Nuclei Recovery	Total cDNA Yield (ng)	cDNA Input into Fragmentation		SI PCR Cycle Number
			Volume ( $\mu\text{l}$ )	Mass (ng)	
High RNA Content 	Low 	150 ng	10 $\mu\text{l}$	37.5 ng	14
	High 	400 ng	10 $\mu\text{l}$	100 ng	13
Low RNA Content 	Low 	1 ng	10 $\mu\text{l}$	0.25 ng	16
	High 	100 ng	10 $\mu\text{l}$	25 ng	14

## 7.1 Fragmentation, End Repair & A-tailing

- a. Prepare a thermal cycler with the following incubation protocol.



Lid Temperature	Reaction Volume	Run Time hh:mm:ss
65°C	50 µl	~35 min
Step	Temperature	Time
Pre-cool block <i>Pre-cool block prior to preparing the Fragmentation Mix</i>	4°C	Hold
Fragmentation	32°C	00:05:00
End Repair & A-tailing	65°C	00:30:00
Hold	4°C	Hold

- b. Vortex Fragmentation Buffer. Verify there is no precipitate.

- c. Prepare Fragmentation Mix on ice. Pipette mix and centrifuge briefly.

Fragmentation Mix <i>Add reagents in the order listed</i>	PN	1X (µl)	4X + 10% (µl)	8X + 10% (µl)
● Fragmentation Buffer	2000091	5	22	44
● Fragmentation Enzyme	2000090/ 2000104	10	44	88
<b>Total</b>	-	<b>15</b>	<b>66</b>	<b>132</b>

- d. Transfer **ONLY 10 µl** purified cDNA sample from cDNA Cleanup (step 6.2n) to a tube strip.

Note that only **10 µl** (25%) cDNA sample is sufficient for generating 3' Gene Expression library. The remaining **30 µl** (75%) cDNA sample can be stored at **4°C** for up to **72 h** or at **-20°C** for up to **4 weeks** for generating additional Gene Expression libraries.

- e. Add **25 µl** Buffer EB to each sample.

- f. Add **15 µl** Fragmentation Mix to each sample.

- g. Pipette mix 15x (pipette set to 35 µl) on ice. Centrifuge briefly.

- h. Transfer into the pre-cooled thermal cycler (**4°C**) and press "SKIP" to initiate the protocol.

7.2  
Post Fragmentation,  
End Repair & A-tailing  
Double Sided Size  
Selection – SPRIselect

- a. Vortex to resuspend SPRIselect reagent. Add **30 µl SPRIselect (0.6X)** reagent to each sample. Pipette mix 15x (pipette set to 75 µl).
- b. Incubate **5 min at room temperature**.
- c. Place on the magnet•**High** until the solution clears. DO NOT discard supernatant.
- d. Transfer **75 µl** supernatant to a new tube strip.
- e. Vortex to resuspend SPRIselect reagent. Add **10 µl SPRIselect reagent (0.8X)** to each sample. Pipette mix 15x (pipette set to 80 µl).
- f. Incubate **5 min at room temperature**.
- g. Place on the magnet•**High** until the solution clears.
- h. Remove **80 µl** supernatant. DO NOT discard any beads.
- i. Add **125 µl 80% ethanol** to the pellet. Wait **30 sec**.
- j. Remove the ethanol.
- k. **Repeat** steps i and j for a total of 2 washes.
- l. Centrifuge briefly. Place on the magnet•**Low** until the solution clears. Remove remaining ethanol. Air dry for **2 min**. DO NOT exceed **2 min** as this will decrease elution efficiency.
- m. Remove from the magnet. Add **50.5 µl Buffer EB** to each sample. Pipette mix 15x.
- n. Incubate **2 min at room temperature**.
- o. Place on the magnet•**High** until the solution clears.
- p. Transfer **50 µl** sample to a new tube strip.

### 7.3 Adaptor Ligation

a. Prepare Adaptor Ligation Mix. Pipette mix and centrifuge briefly.

Adaptor Ligation Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
● Ligation Buffer	2000092	20	88	176
● DNA Ligase	220110/ 220131	10	44	88
● Adaptor Oligos	2000094	20	88	176
<b>Total</b>	-	<b>50</b>	<b>220</b>	<b>440</b>

b. Add 50 μl Adaptor Ligation Mix to 50 μl sample. Pipette mix 15x (pipette set to 90 μl). Centrifuge briefly.

c. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time hh:mm:ss
30°C	100 μl	15 min
Step	Temperature	Time
1	20°C	00:15:00
2	4°C	Hold

#### 7.4 Post Ligation Cleanup – SPRIselect

- a. Vortex to resuspend SPRIselect Reagent. Add **80 µl** SPRIselect Reagent (**0.8X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears.
- d. Remove the supernatant.
- e. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- f. Remove the ethanol.
- g. **Repeat** steps e and f for a total of 2 washes.
- h. Centrifuge briefly. Place on the magnet•**Low**.
- i. Remove any remaining ethanol. Air dry for **2 min**. **DO NOT** exceed **2 min** as this will decrease elution efficiency.
- j. Remove from the magnet. Add **30.5 µl** Buffer EB. Pipette mix 15x.
- k. Incubate **2 min** at **room temperature**.
- l. Place on the magnet•**Low** until the solution clears.
- m. Transfer **30 µl** sample to a new tube strip.

## 7.5 Sample Index PCR



- a. Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run. Record the 10x sample index name (PN-3000431 Dual Index Plate TT Set A well ID) used.
- b. Add **50 µl** Amp Mix (PN-2000047/2000131) to **30 µl** sample.
- c. Add **20 µl** of an individual Dual Index TT Set A to each well and record the well ID used. Pipette mix 5x (pipette set to 90 µl). Centrifuge briefly.
- d. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time hh:mm:ss
105°C	100 µl	~25-40 min

Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	54°C	00:00:30
4	72°C	00:00:20
5	Go to step 2, see below for # of cycles	
6	72°C	00:01:00
7	4°C	Hold



The total cycles should be optimized based on 25% carry forward cDNA yield/input calculated during Post cDNA Amplification QC & Quantification (step 6.3)

**e.**

Recommended cycle numbers	
cDNA Input	Total Cycles
0.25-25 ng	14-16
25-150 ng	12-14
150-500 ng	10-12
500-1,000 ng	8-10
1,000-1,500 ng	6-8
>1500 ng	5



- e. Store at **4°C** for up to **72 h** or proceed to the next step.




7.6  
Post Sample Index  
PCR Double Sided Size  
Selection – SPRIselect

- a. Vortex to resuspend the SPRIselect reagent. Add **60 µl** SPRIselect Reagent (**0.6X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears. **DO NOT** discard supernatant.
- d. Transfer **150 µl** supernatant to a new tube strip.
- e. Vortex to resuspend the SPRIselect reagent. Add **20 µl** SPRIselect Reagent (**0.8X**) to each sample (supernatant). Pipette mix 15x (pipette set to 150 µl).
- f. Incubate **5 min** at **room temperature**.
- g. Place the magnet•**High** until the solution clears.
- h. Remove **165 µl** supernatant. **DO NOT** discard any beads.
- i. With the tube still in the magnet, add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- j. Remove the ethanol.
- k. **Repeat** steps i and j for a total of 2 washes.
- l. Centrifuge briefly. Place on the magnet•**Low**. Remove remaining ethanol. Air dry for **2 min**. **DO NOT** exceed **2 min** as this will decrease elution efficiency.
- m. Remove from the magnet. Add **35.5 µl** Buffer EB. Pipette mix 15x.
- n. Incubate **2 min** at **room temperature**.
- o. Place on the magnet•**Low** until the solution clears.
- p. Transfer **35 µl** to a new tube strip.
- q. Store at **4°C** for up to **72 h** or at **-20°C** for **long-term** storage.



## 7.7 Post Library Construction QC

Run 1  $\mu\text{l}$  sample at 1:3 dilution on an Agilent Bioanalyzer High Sensitivity chip.

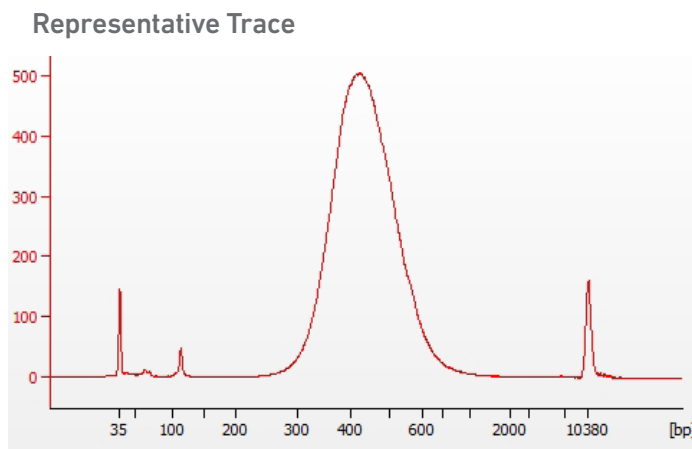


Determine the average fragment size from the Bioanalyzer trace. This will be used as the insert size for library quantification.

**Alternate QC Methods** ([See Appendix for representative traces](#))

- Agilent TapeStation
- LabChip

[See Appendix for Post Library Construction Quantification](#)


# Sequencing

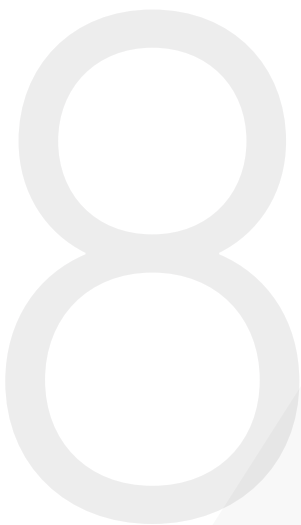

## Sequencing Libraries


Chromium Single Cell Multiome ATAC libraries comprise double stranded DNA with standard Illumina® paired-end constructs which begin with P5 and end with P7. Sequencing these libraries produces a standard Illumina® BCL data output folder that includes paired-end Read 1N and Read 2N used for sequencing the DNA insert, 8 bp sample index in the i7 read, and 24 bp in the i5 read to cover the 16 bp 10x Barcode and 8 bp Spacer.

Chromium Single Cell Multiome ATAC Library

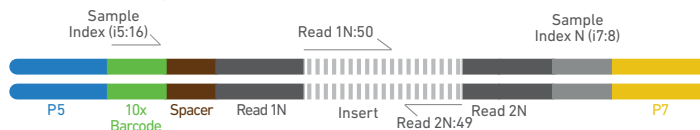

Chromium Single Cell Multiome Gene Expression libraries comprise cDNA insert with standard Illumina® paired-end constructs which begin with P5 and end with P7. Sequencing these libraries produces a standard Illumina® BCL data output folder. TruSeq Read 1 is used to sequence 16 bp 10x Barcodes and 12 bp UMI, while 10 bp i5 and i7 sample index sequences are the sample index reads. TruSeq Read 2 is used to sequence the insert.

Chromium Single Cell Multiome Gene Expression Library

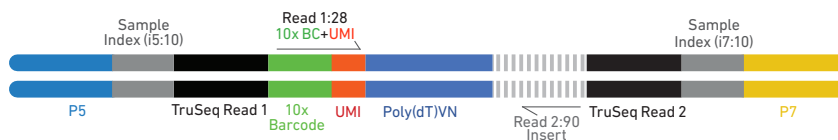

## Illumina® Sequencer Compatibility

The compatibility of the listed sequencers has been verified by 10x Genomics. Some variation in assay performance is expected based on sequencer choice. For more information about performance variation, visit the 10x Genomics Support website.

- MiSeq™
- NextSeq™ 500/550 (High Output)
- NextSeq™ 1000/2000
- HiSeq 2500™ (Rapid Run)
- HiSeq™ 3000/4000
- NovaSeq™

## Sample Indices

Each sample index in the Dual Index Kit TT Set A (PN-1000215) is a mix of one unique i7 and one unique i5 sample index. Each i7 sample index in the Single Index Kit N Set A (PN-1000212) is a mix of 4 different sequences to balance across all 4 nucleotides. If multiple samples are pooled in a sequence lane, the sample index name (i.e. Single Index Plate\_Set\_well ID) is needed in the sample sheet used for generating FASTQs with Cell Ranger. Samples utilizing the same sample index should not be pooled together or run on the same flow cell lane, as this would not enable correct sample demultiplexing.

## ATAC Library Sequencing Depth & Run Parameters



These sequencing parameters are specific for Chromium Single Cell Multiome ATAC libraries and are different from the recommendations for standalone ATAC libraries. Ensure that these specific recommendations are provided to the sequencing service provider.

<b>Sequencing Depth</b>	25,000 read pairs per nucleus (25,000 reads for Read 1N; 25,000 reads for Read 2N)
<b>Sequencing Type</b>	Paired-end, dual indexing
<b>Sequencing Read</b>	
Read 1N	50 cycles
i7 Index	8 cycles
i5 Index	24 cycles*
Read 2N	49 cycles



### \*Custom sequencing recipe:

Sequencers that do not support 24 nt read in i5 (e.g. NextSeq™ 500/550) require a custom recipe that includes 8 dark cycles and 16 nt cycles on i5. After installation of custom sequencing recipe, input 16 cycles for i5 read.

It is **imperative to use a custom recipe** for these sequencers. Entering 16 cycles for i5 read without the use of the custom recipe will cause the sequencing run to proceed but the data will be unusable.

Custom recipe is NOT required for NextSeq™ 1000/2000.

Contact [Support@10xgenomics.com](mailto:Support@10xgenomics.com) for any additional questions.

## ATAC Library Loading

Once quantified and normalized, ATAC libraries should be denatured and diluted according to the table below. Consult the Technical Note on Sequencing Metrics and Base Composition of Single Cell Multiome ATAC Libraries (CG000373), available at the 10x Genomics Support website, for more information.

Instrument	Loading Concentration (pM)	PhiX (%)
MiSeq™	10	1
NextSeq™ 500/550	1.5	1
NextSeq™ 1000/2000	650	1
HiSeq™ 2500 (RR)	10	1
HiSeq™ 4000	180	1
NovaSeq™	300	1

### Gene Expression Library Sequencing Depth & Run Parameters

<b>Sequencing Depth</b>	20,000 read pairs per nucleus
<b>Sequencing Type</b>	Paired-end, dual indexing
<b>Sequencing Read</b>	Recommended Cycles
Read 1	28 cycles
i7 Index	10 cycles
i5 Index	10 cycles
Read 2	90 cycles

### Gene Expression Library Loading

Once quantified and normalized, libraries should be denatured and diluted according to the table below. Refer to Illumina® documentation for denaturing and diluting libraries. As the Multiome Gene Expression library is same as the Chromium Single Cell 3' Gene Expression Dual Index library, consult the Technical Note on Sequencing Metrics & Base Composition of Single Cell 3' v3.1 Dual Index Libraries (CG000374), available at the 10x Genomics Support website, for more information.

Instrument	Loading Concentration (pM)	PhiX (%)
MiSeq™	11	1
NextSeq™ 500/550	1.8	1
NextSeq™ 1000/2000	650	1
HiSeq™ 2500 (RR)	11	1
HiSeq™ 4000	240	1
NovaSeq™	150*/300	1

\*Use 150pM loading concentration for Illumina XP workflow

### Library Pooling

Single Cell Multiome ATAC libraries maybe pooled with other ATAC libraries only when using forward strand Illumina® workflow. Single Cell Multiome Gene Expression libraries maybe pooled for sequencing with other libraries, taking into account the differences in cell number and per-cell read depth requirements between each library. Samples utilizing the same sample index should not be pooled together, or run on the same flow cell lane, as this would not enable correct sample demultiplexing. Refer to the 10x Genomics Support website for more information.

# Troubleshooting



GEMs

STEP	NORMAL	REAGENT CLOGS & WETTING FAILURES
------	--------	----------------------------------

2.4 d  
After Chip J is removed from the Controller and the wells are exposed




All 8 recovery wells are similar in volume and opacity.




Recovery well G indicates a reagent clog. Recovery well C and E indicate a wetting failure. Recovery wells B, D, and F are normal. Wells A and H contain 50% Glycerol Solution.

2.4 e  
Transfer GEMs from Chip J Row Labeled 3

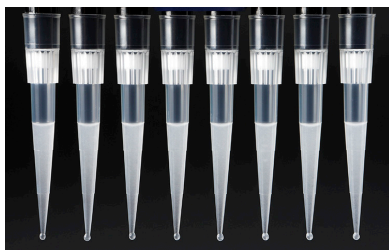

All liquid levels are similar in volume and opacity without air trapped in the pipette tips.

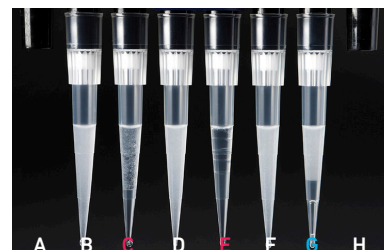


Pipette tips C and E indicate a wetting failure. Pipette tip C contains partially emulsified GEMs. Emulsion is absent in pipette tip E. Pipette tip G indicates a reagent clog.




STEP	NORMAL	REAGENT CLOGS & WETTING FAILURES
------	--------	----------------------------------

3.1 a  
After transfer of the  
GEMs +  
Recovery Agent

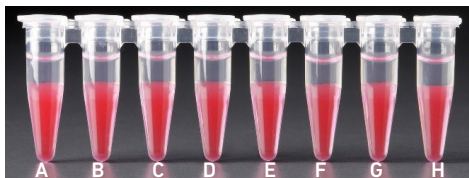

All liquid levels are similar in the aqueous sample volume (clear) and Recovery Agent/Partitioning Oil (pink).

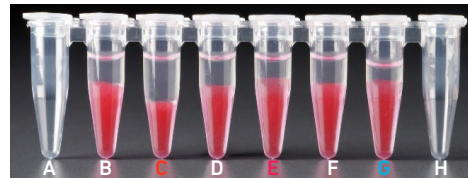

Tube **G** indicates a reagent clog has occurred. There is a decreased volume of aqueous layer (clear).  
Tube **C** and **E** indicate a wetting failure has occurred. There is an abnormal volume of Recovery Agent/Partitioning Oil (pink).

3.1 b  
After aspiration of  
Recovery Agent/  
Partitioning Oil



All liquid volumes are similar in the aqueous sample volume (clear) and residual Recovery Agent/Partitioning Oil (pink).



Tube **G** indicates a reagent clog has occurred. There is a decreased volume of aqueous layer (clear). There is also a greater residual volume of Recovery Agent/Partitioning Oil (pink).  
Tube **C** and **E** indicate a wetting failure has occurred. There is an abnormal residual volume of Recovery Agent/Partitioning Oil (pink).

3.1 d  
After addition of  
Dynabeads  
Cleanup Mix



All liquid volumes are similar after addition of the Dynabeads Cleanup Mix.



Tube **G** indicates a reagent clog has occurred. There is an abnormal ratio of Dynabeads Cleanup Mix (brown) to Recovery Agent/Partitioning Oil (appears white).  
Tube **C** and **E** indicate a wetting failure has occurred. There is an abnormal ratio of Dynabeads Cleanup Mix (brown) to Recovery Agent/Partitioning Oil (appears white).

If a channel clogs or wetting failure occurs during GEM generation, it is recommended that the sample be remade.  
If any of the listed issues occur, take a picture and send it to [support@10xgenomics.com](mailto:support@10xgenomics.com) for further assistance.

## Chromium Controller Errors

If the Chromium Controller or the Chromium Single Cell Controller fails to start, an error tone will sound and one of the following error messages will be displayed:

- a. **Chip not read – Try again:** Eject the tray, remove and/or reposition the Chromium Next GEM Secondary Holder assembly and try again. If the error message is still received after trying this more than twice, contact [support@10xgenomics.com](mailto:support@10xgenomics.com) for further assistance.
- b. **Check gasket:** Eject the tray by pressing the eject button to check that the 10x Gasket is correctly installed on the Chromium Next GEM Chip. If the error message persists, contact [support@10xgenomics.com](mailto:support@10xgenomics.com) for further assistance.
- c. **Error Detected: Row \_ Pressure:**
  - i. If this message is received within a few seconds of starting a run, eject the tray by pressing the eject button and check for dirt or deposits on the 10x Gasket. If dirt is observed, replace with a new 10x Gasket and try again. If the error message is still received after trying this more than twice, contact [support@10xgenomics.com](mailto:support@10xgenomics.com) for further assistance.
  - ii. If this message is received after a few minutes into the run, the Chromium Next GEM Chip must be discarded. **Do not try running this Chromium Next GEM Chip again as this may damage the Chromium Controller.**
- d. **Invalid Chip CRC Value:** This indicates that a Chromium Next GEM Chip has been used with an older firmware version. The chip must be discarded. Contact [support@10xgenomics.com](mailto:support@10xgenomics.com) for further assistance.
- e. **Chip Holder Not Present:** Open the controller drawer and check if chip holder is present. Insert chip properly into chip holder and retry.
- f. **Unauthorized Chip:** This indicates that an incompatible non-Next GEM chip has been used with an instrument that only can run Next GEM assays. Use only Chromium Controller (PN-120223;120246) or Chromium Single Cell Controller (PN-120263;120212) to run that chip or chip must be discarded. Contact [support@10xgenomics.com](mailto:support@10xgenomics.com) for further assistance.
- g. **Endpoint Reached Early:** If this message is received, contact [support@10xgenomics.com](mailto:support@10xgenomics.com) for further assistance.

# Appendix

Post Library Construction Quantification

Agilent TapeStation Traces

LabChip Traces

Assay Scheme Overview

Sequences

## Post Library Construction Quantification

- Thaw KAPA Library Quantification Kit for Illumina Platforms.
- Dilute **2  $\mu$ l** sample with deionized water to appropriate dilutions that fall within the linear detection range of the KAPA Library Quantification Kit for Illumina Platforms. (For more accurate quantification, make the dilution(s) in duplicate).
- Make enough Quantification Master Mix for the DNA dilutions per sample and the DNA Standards (plus 10% excess) using the guidance for 1 reaction volume below.

Quantification Master Mix	1X ( $\mu$ l)
SYBR Fast Master Mix + Primer	12
Water	4
<b>Total</b>	<b>16</b>

- Dispense **16  $\mu$ l** Quantification Master Mix for sample dilutions and DNA Standards into a 96 well PCR plate.
- Add **4  $\mu$ l** sample dilutions and **4  $\mu$ l** DNA Standards to appropriate wells. Centrifuge briefly.
- Incubate in a thermal cycler with the following protocol.

Step	Temperature	Run Time
1	95°C	00:03:00
2	95°C	00:00:05
3	67°C	00:00:30
4	Go to Step 2, 29X (Total 30 cycles)	

- Follow the manufacturer's recommendations for qPCR-based quantification. For library quantification for sequencer clustering, determine the concentration based on insert size derived from the Bioanalyzer/TapeStation trace.

## Agilent TapeStation Traces


### Agilent TapeStation Traces

Agilent TapeStation High Sensitivity D5000 ScreenTape was used.

Protocol steps correspond to the Chromium Next GEM Single Cell Multiome ATAC + Gene Expression User Guide (CG000338).


#### Protocol Step 5.3 – Post Library Construction QC (ATAC Library)

Run 2  $\mu$ l sample

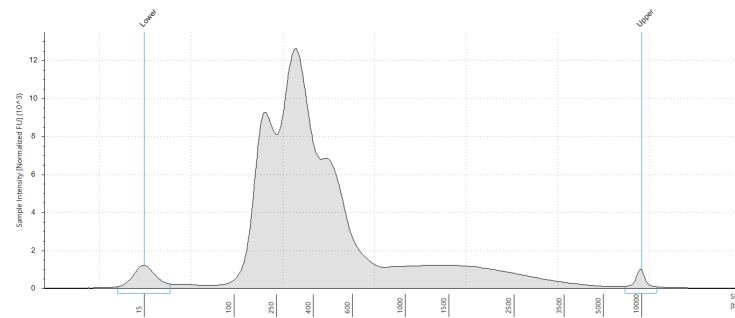


#### Protocol Step 6.3 – cDNA QC & Quantification

Run 2  $\mu$ l sample

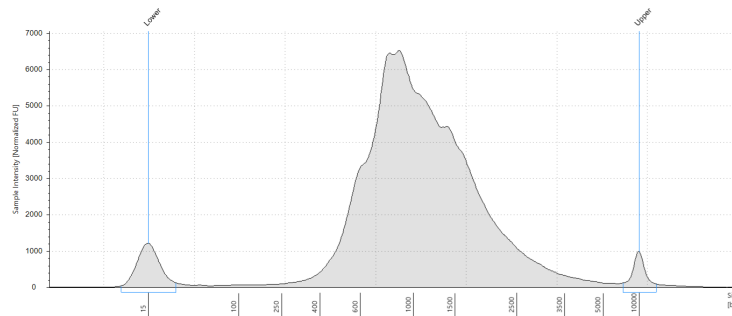

#### Protocol Step 7.7 – Post Library Construction QC (Gene Expression Library)

Run 2  $\mu$ l sample

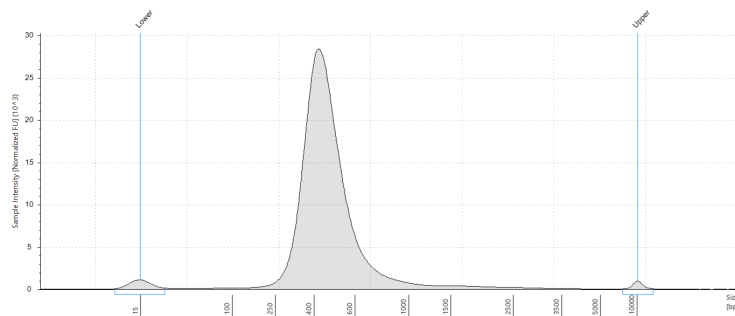

All traces are representative.

## LabChip Traces


### LabChip Traces

DNA High Sensitivity Reagent Kit was used.

Protocol steps correspond to the Chromium Next GEM Single Cell Multiome ATAC + Gene Expression User Guide (CG000338).


#### Protocol Step 5.3 – Post Library Construction QC (ATAC Library)

Run 10  $\mu$ l undiluted sample

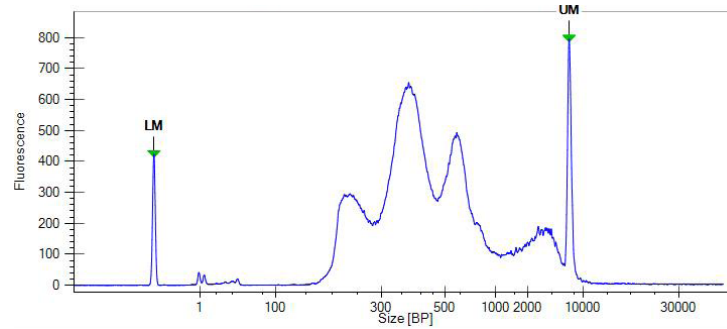


#### Protocol Step 6.3 – cDNA QC & Quantification

Run 10  $\mu$ l undiluted sample

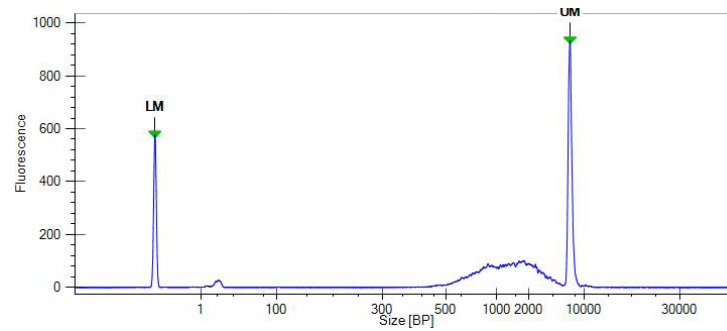


#### Protocol Step 7.7 – Post Library Construction QC (Gene Expression Library)

Run 10  $\mu$ l undiluted sample

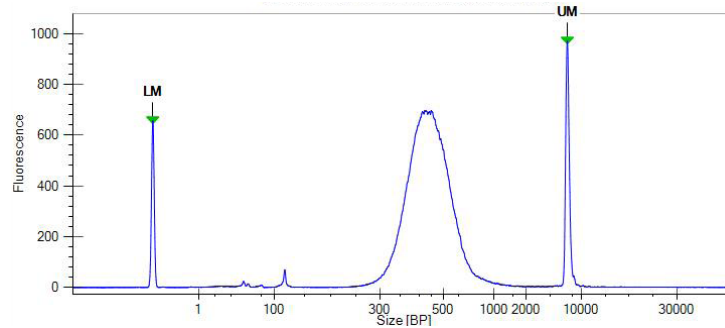

All traces are representative.

Assay Scheme Overview

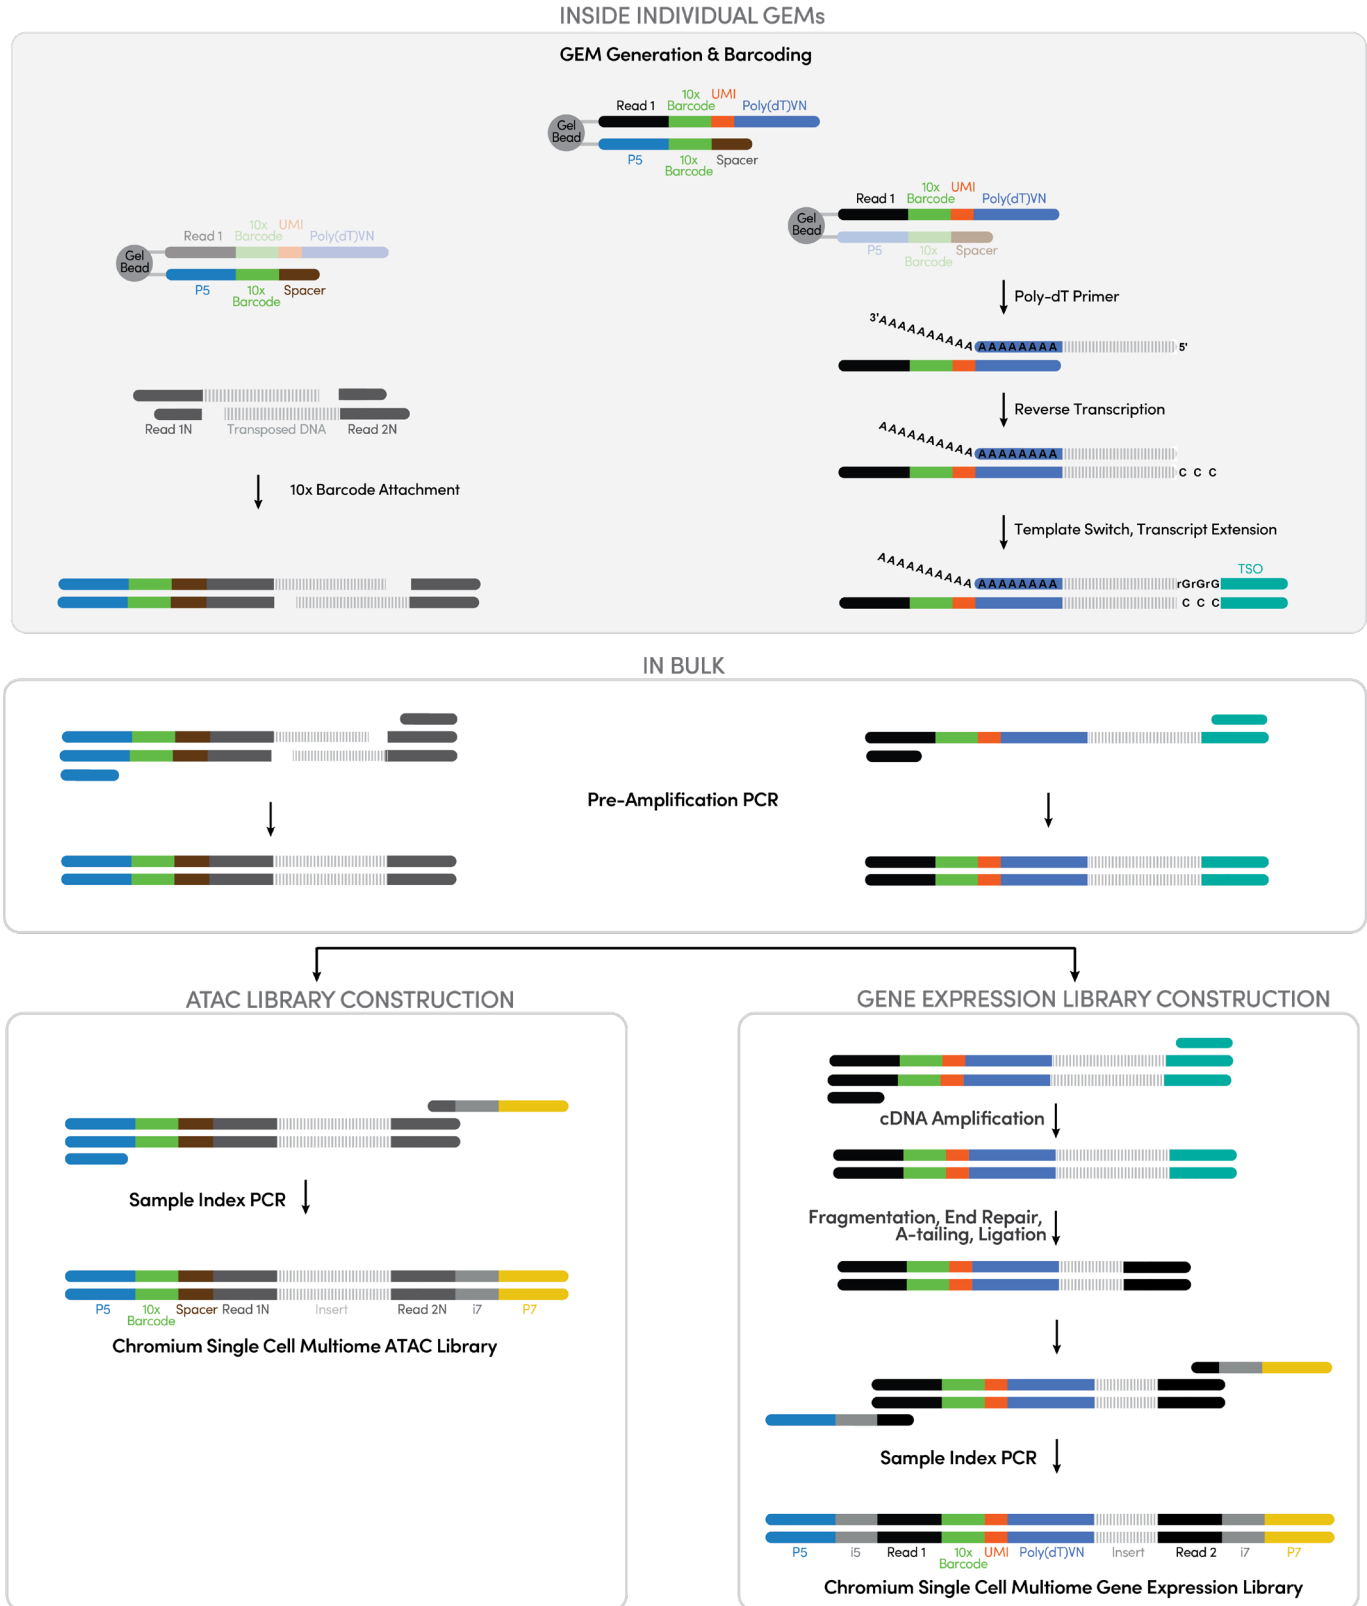

## Sequences

### Single Cell Multiome Gel Beads A (PN- 2000261)

5'-CTACACGACGCTCTCCGATCT-N16-N12-TTTTTTTTTTTTTTTTTTTTTTTTTTTTTTTTTT-VN-3'




5'-AATGATACGGCGACCACCGAGATCTACAC-N16-CGCGTCTG-3'

### Chromium Single Cell Multiome ATAC Library



5'-AATGATACGGCGACCACCGAGATCTACAC-N16-CGCGTCTG-TCGTCGGCAGCGTCAGATGTGTATAAGAGACAG---insert---CTGTCTCTTATACATCTCCGAGCCACGAGAC-N8-ATCTCGTATGCCGTCTTCTGCTTG-3'  
 3'-TTACTATGCCGTGGTGGCTCTAGATGTC-N16-GCGCAGAC-AGCAGCCGTCGCAGTCTACACATATTCTCTGTCTC---insert---GACAGAGAATATGTGTAGAGGCTCGGGTCTCTG-N8-TAGAGCATACGGCAGAAAGACGAAC-5'

### Chromium Single Cell Multiome Gene Expression Library



5'-AATGATACGGCGACCACCGAGATCTACAC-N10-ACACTCTTTCCCTACACGACGCTCTCCGATCT-N16-N12-TTTTTTTTTTTTTTTTTTTTTTTTTTTTTTTTTT-VN-cDNA\_Insert-AGATCGGAAGAGCACACGTCTGAACTCCAGTCAC-N10-ATCTCGTATGCCGTCTTCTGCTTG-3'  
 3'-TTACTATGCCGTGGTGGCTCTAGATGTC-N10-TGTGAGAAAGGGATGTGCTGCGAGAAGGCTAGA-N16-N12-AAAAAAAAAAAAAAAAAAAAAAAAAAAAAAAAABN-cDNA\_Insert-TCTAGCCTTCTCGTGTGCAGACTTGAGGTCAAGT-N10-TAGAGCATACGGCAGAAAGACGAAC-5'