

USER GUIDE

Chromium Next GEM Single Cell V(D)J Reagent Kits v1.1

with Feature Barcoding technology for
Cell Surface Protein



FOR USE WITH

Chromium Next GEM Single Cell 5' Library & Gel Bead Kit v1.1, 16 rxns PN-1000165

Chromium Next GEM Single Cell 5' Library & Gel Bead Kit v1.1, 4 rxns PN-1000167

Chromium Single Cell 5' Library Construction Kit, 16 rxns PN-1000020

Chromium Single Cell 5' Feature Barcode Library Kit, 16 rxns PN-1000080

Chromium Single Cell V(D)J Enrichment Kit, Human T Cell, 96 rxns PN-1000005

Chromium Single Cell V(D)J Enrichment Kit, Human B Cell, 96 rxns PN-1000016

Chromium Single Cell V(D)J Enrichment Kit, Mouse T Cell, 96 rxns PN-1000071

Chromium Single Cell V(D)J Enrichment Kit, Mouse B Cell, 96 rxns PN-1000072

Chromium Next GEM Chip G Single Cell Kit, 48 rxns PN-1000120

Chromium Next GEM Chip G Single Cell Kit, 16 rxns PN-1000127

Chromium i7 Multiplex Kit, 96 rxns PN-120262

Chromium i7 Multiplex Kit N, Set A, 96 rxn PN-1000084

Notices

Document Number

CG000208 • Rev B

Legal Notices

© 2019 10X Genomics, Inc. (10x Genomics). All rights reserved. Duplication and/or reproduction of all or any portion of this document without the express written consent of 10x Genomics, is strictly forbidden. Nothing contained herein shall constitute any warranty, express or implied, as to the performance of any products described herein. Any and all warranties applicable to any products are set forth in the applicable terms and conditions of sale accompanying the purchase of such product. 10x Genomics provides no warranty and hereby disclaims any and all warranties as to the use of any third-party products or protocols described herein. The use of products described herein is subject to certain restrictions as set forth in the applicable terms and conditions of sale accompanying the purchase of such product. A non-exhaustive list of 10x Genomics' marks, many of which are registered in the United States and other countries can be viewed at: www.10xgenomics.com/trademarks. 10x Genomics may refer to the products or services offered by other companies by their brand name or company name solely for clarity, and does not claim any rights in those third-party marks or names. 10x Genomics products may be covered by one or more of the patents as indicated at: www.10xgenomics.com/patents. The use of products described herein is subject to 10x Genomics Terms and Conditions of Sale, available at www.10xgenomics.com/legal-notices, or such other terms that have been agreed to in writing between 10x Genomics and user. All products and services described herein are intended FOR RESEARCH USE ONLY and NOT FOR USE IN DIAGNOSTIC PROCEDURES.

Instrument & Licensed Software Updates Warranties

Updates to existing Instruments and Licensed Software may be required to enable customers to use new or existing products. In the event of an Instrument failure resulting from an update, such failed Instrument will be replaced or repaired in accordance with the 10x Limited Warranty, Assurance Plan or service agreement, only if such Instrument is covered by any of the foregoing at the time of such failure. Instruments not covered under a current 10x Limited Warranty, Assurance Plan or service agreement will not be replaced or repaired.

Support

Email: support@10xgenomics.com

10x Genomics

7068 Koll Center Parkway

Suite 401

Pleasanton, CA 94566 USA

Document Revision Summary

Document Number CG000208

Title Chromium Next GEM Single Cell V(D)J Reagent Kits v1.1
User Guide with Feature Barcoding technology for Cell
Surface Protein

Revision Rev A to Rev B

Revision Date June 2019

Specific Changes:

- Updated to include part number for kit containing the Chromium Next GEM Secondary Holder
- Updated information regarding Chromium Controller Errors

Table of Contents

Introduction	6
Chromium Next GEM Single Cell V(D)J Reagent Kits v1.1	7
Chromium Accessories	12
Recommended Thermal Cyclers	12
Additional Kits, Reagents & Equipment	13
Protocol Steps & Timing	15
Stepwise Objectives	16
Cell Surface Protein Labeling Guidelines	21
Tips & Best Practices	22
Step 1	29
GEM Generation & Barcoding	30
1.1 Prepare Reaction Mix	31
1.2 Load Chromium Next GEM Chip G	33
1.3 Run the Chromium Controller	34
1.4 Transfer GEMs	34
1.5 GEM-RT Incubation	35
Step 2	36
Post GEM-RT Cleanup	37
2.1 Post GEM-RT Cleanup – Dynabeads	38
Step 3	40
cDNA Amplification & QC	41
3.1 cDNA Amplification	42
Step Overview (steps 3.1 & 3.2)	43
3.2 cDNA Cleanup – SPRIselect	44
3.2A Pellet Cleanup (for V(D)J Enriched & 5' Gene Expression library)	44
3.2B Transferred Supernatant Cleanup (for Cell Surface Protein library)	44
3.3 cDNA QC & Quantification	45
Step 4	46
Target Enrichment from cDNA	47
4.1 Target Enrichment 1	48
4.2 Post Target Enrichment 1 Cleanup – SPRIselect	49
4.3 Target Enrichment 2	50
4.4 Post Target Enrichment 2 Double Sided Size Selection – SPRIselect	51
4.5 Post Target Enrichment QC & Quantification	52

Step 5	53
Enriched Library Construction	54
5.1 Fragmentation, End Repair & A-tailing	55
5.2 Adaptor Ligation	56
5.3 Post Ligation Cleanup – SPRIselect	57
5.4 Sample Index PCR	58
5.5 Post Sample Index PCR Cleanup – SPRIselect	59
5.6 Post Library Construction QC	60
Step 6	61
5' Gene Expression (GEX) Library Construction	62
6.1 GEX Fragmentation, End Repair & A-tailing	63
6.2 GEX Post Fragmentation, End Repair & A-tailing Double Sided Size Selection – SPRIselect	64
6.3 GEX Adaptor Ligation	65
6.4 GEX Post Ligation Cleanup – SPRIselect	66
6.5 GEX Sample Index PCR	67
6.6 GEX Post Sample Index PCR Double Sided Size Selection – SPRIselect	68
6.7 GEX Post Library Construction QC	69
Step 7	70
Cell Surface Protein Library Construction	71
7.1 Sample Index PCR	72
7.2 Post Sample Index PCR Size Selection – SPRIselect	73
7.3 Post Library Construction QC	74
Sequencing	75
Troubleshooting	78
GEMs	79
Chromium Controller Errors	81
Appendix	82
Post Library Construction Quantification	83
Agilent TapeStation Traces	84
Oligonucleotide Sequences	85

Introduction

Chromium Next GEM Single Cell V(D)J Reagent Kits v1.1

Chromium Accessories

Recommended Thermal Cyclers

Additional Kits, Reagents & Equipments

Protocol Steps & Timing









Stepwise Objectives








Cell Surface Protein Labeling Guidelines

Chromium Next GEM Single Cell V(D)J Reagent Kits v1.1

Chromium Next GEM Single Cell 5' Library and Gel Bead Kit v1.1, 16 rxns PN-1000165

Chromium Next GEM Single Cell 5' Library Kit v1.1, 16 rxns PN-1000166 (store at –20°C)

Chromium Next GEM Single Cell 5' Reagents Module 1 v1.1			#	PN
 RT Reagent B			1	2000165
 RT Enzyme Mix B			1	2000010
 Additive A			1	220074
 Poly-dT RT Primer			1	2000007
 Buffer Sample Clean Up 1			2	220020
 Amplification Master Mix			2	220125
 cDNA Primer Mix			1	220106
 cDNA Additive			1	220067

Chromium Next GEM Single Cell 5' Reagents Module 2 v1.1			#	PN
 Fragmentation Enzyme Blend			1	220107
 Fragmentation Buffer			1	220108
 Ligation Buffer			1	220109
 DNA Ligase			1	220110
 Adaptor Mix			1	220026
 SI-PCR Primer			1	220111
 Amplification Master Mix			1	220125

Chromium Next GEM Single Cell 5' Gel Bead Kit v1.1, 16 rxns PN-1000169 (store at –80°C)

Chromium Next GEM Single Cell 5' Gel Beads v1.1			#	PN
Single Cell VDJ 5' Gel Beads v1.1			2	2000209

Dynabeads™ MyOne™ SILANE PN-2000048 (store at 4°C)

	#	PN
Dynabeads MyOne SILANE	1	2000048

Chromium Next GEM Single Cell 5' Library and Gel Bead Kit v1.1, 4 rxns PN-1000167

Chromium Next GEM Single Cell 5' Library Kit v1.1, 4 rxns PN-1000168 (store at -20°C)

Chromium Next GEM Single Cell 5' Reagents Module 1 v1.1			Chromium Next GEM Single Cell 5' Reagents Module 2 v1.1		
	#	PN		#	PN
● RT Reagent B	1	2000165	● Fragmentation Enzyme Blend	1	220130
○ RT Enzyme Mix B	1	2000021	○ Fragmentation Buffer	1	220108
● Additive A	1	220074	● Ligation Buffer	1	220109
● Poly-dT RT Primer	1	2000007	● DNA Ligase	1	220131
● Buffer Sample Clean Up 1	1	220020	● Adaptor Mix	1	220026
● Amplification Master Mix	1	220125	● SI-PCR Primer	1	220111
● cDNA Primer Mix	1	220106			
● cDNA Additive	1	220067			
10xGenomics.com			10xGenomics.com		
10x GENOMICS			10x GENOMICS		









Chromium Next GEM Single Cell 5' Gel Bead Kit v1.1, 4 rxns PN-1000170 (store at -80°C)

Chromium Next GEM Single Cell 5' Gel Beads v1.1		
	#	PN
Single Cell VDJ 5' Gel Beads v1.1	1	2000209
10xGenomics.com		
10x GENOMICS		

Dynabeads™ MyOne™ SILANE PN-2000048 (store at 4°C)

	#	PN
Dynabeads MyOne SILANE	1	2000048




Chromium Single Cell 5' Library Construction Kit, 16 rxns PN-1000020 (store at -20°C)

Chromium Single Cell 5' Library Construction kit		
	#	PN
 cDNA Additive	2	220067
 Fragmentation Enzyme Blend	1	220107
 Fragmentation Buffer	1	220108
 Ligation Buffer	1	220109
 DNA Ligase	1	220110
 Amplification Master Mix	3	220125
 Adapter Mix	1	220026
 SI-PCR Primer	1	220111

10xGenomics.com

10x
GENOMICS

Chromium Single Cell 5' Feature Barcode Library Kit, 16 rxns PN-1000080 (store at -20°C)

Chromium Single Cell 5' Feature Barcode Library Kit		
	#	PN
 SC5' Feature cDNA Primers	1	2000119
 Amplification Master Mix	1	220125
 SI Primer	1	2000095

10xGenomics.com

10x
GENOMICS

Chromium Single Cell V(D)J Enrichment Kits, Human (store at –20°C)

Human T Cell, 96 rxns PN-1000005

Chromium
Single Cell V(D)J Enrichment Kit
Human T Cell

	#	PN
● Human T Cell Mix 1	6	2000008
● Human T Cell Mix 2	6	2000009

10xGenomics.com 10x GENOMICS

Human B Cell, 96 rxns PN-1000016

Chromium
Single Cell V(D)J Enrichment Kit
Human B Cell

	#	PN
● Human B Cell Mix 1	6	2000035
● Human B Cell Mix 2	6	2000036

10xGenomics.com 10x GENOMICS

Chromium Single Cell V(D)J Enrichment Kits, Mouse (store at –20°C)

Mouse T Cell, 96 rxns PN-1000071

Chromium
Single Cell V(D)J Enrichment Kit
Mouse T Cell

	#	PN
● Mouse T Cell Mix 1	6	2000075
● Mouse T Cell Mix 2	6	2000079

10xGenomics.com 10x GENOMICS

Mouse B Cell, 96 rxns PN-1000072

Chromium
Single Cell V(D)J Enrichment Kit
Mouse B Cell

	#	PN
● Mouse B Cell Mix 1	6	2000080
● Mouse B Cell Mix 2	6	2000081

10xGenomics.com 10x GENOMICS

Chromium Next GEM Chip G Single Cell Kit, 48 rxns PN-1000120 (store at ambient temperature)

Chromium Partitioning Oil			Chromium Recovery Agent		
	#	PN		#	PN
Partitioning Oil	6	2000190	<input type="radio"/> Recovery Agent	6	220016

Chromium Next GEM Chip G & Gaskets					
	#	PN		#	PN
Chromium Next GEM Chip G	6	2000177			
Gasket, 6-pack	1	370017			

10xGenomics.com **10x** GENOMICS

Chromium Next GEM Chip G Single Cell Kit, 16 rxns PN-1000127 (store at ambient temperature)

Chromium Partitioning Oil			Chromium Recovery Agent		
	#	PN		#	PN
Partitioning Oil	2	2000190	<input type="radio"/> Recovery Agent	2	220016

Chromium Next GEM Chip G & Gaskets					
	#	PN		#	PN
Chromium Next GEM Chip G	2	2000177			
Gasket, 2-pack	1	3000072			

10xGenomics.com **10x** GENOMICS

Chromium i7 Multiplex Kit, 96 rxns PN-120262 (store at -20°C)

Chromium i7 Multiplex Kit					
	#	PN		#	PN
Chromium i7 Sample Index Plate	1	220103			

Chromium i7 Multiplex Kit N, Set A, 96 rxns PN-1000084 (store at -20°C)

Chromium i7 Multiplex Kit N, Set A					
	#	PN		#	PN
Chromium i7 Sample Index Plate N, Set A	1	3000262			

Chromium Accessories

Product	PN (Kit)	PN (Item)
10x Vortex Adapter	120251	330002
Chromium Next GEM Secondary Holder	1000195	3000332
10x Magnetic Separator	120250	230003

Recommended Thermal Cyclers

Thermal cyclers used must support uniform heating of 100 µl emulsion volumes.

Supplier	Description	Part Number
BioRad	C1000 Touch Thermal Cycler with 96-Deep Well Reaction Module	1851197
Eppendorf	MasterCycler Pro	North America 950030010 International 6321 000.019
Thermo Fisher Scientific	Veriti 96-Well Thermal Cycler	4375786

Additional Kits, Reagents & Equipment

The items in the table below have been validated by 10x Genomics and are highly recommended for the Single Cell V(D)J protocols. Substituting materials may adversely affect system performance.

Supplier	Description	Part Number (US)
Plastics		
Eppendorf	PCR Tubes 0.2 ml 8-tube strips DNA LoBind Tubes, 1.5 ml DNA LoBind Tubes, 2.0 ml	Choose either Eppendorf, USA Scientific or Thermo Fisher Scientific PCR 8-tube strips. 951010022 022431021 022431048
USA Scientific	TempAssure PCR 8-tube strip	1402-4700
Thermo Fisher Scientific	MicroAmp 8-Tube Strip, 0.2 ml MicroAmp 8-Cap Strip, clear	N8010580 N8010535
Rainin	Tips LTS 200UL Filter RT-L200FLR Tips LTS 1ML Filter RT-L1000FLR Tips LTS 20UL Filter RT-L10FLR	30389240 30389213 30389226
Kits & Reagents		
Thermo Fisher Scientific	Nuclease-free Water	AM9937
Millipore Sigma	Ethanol, Pure (200 Proof, anhydrous)	E7023-500ML
Beckman Coulter	SPRIselect Reagent Kit	B23318
Bio-Rad	10% Tween 20	1662404
Ricca Chemical Company	Glycerin (glycerol), 50% (v/v) Aqueous Solution	3290-32
Qiagen	Qiagen Buffer EB	19086
Equipment		
VWR	Vortex Mixer Divided Polystyrene Reservoirs	10153-838 41428-958
Eppendorf	Eppendorf ThermoMixer C Eppendorf SmartBlock 1.5 ml, Thermoblock for 24 reaction vessel (alternatively, use a temperature-controlled Heat Block)	5382000023 5360000038
Rainin	Pipet-Lite Multi Pipette L8-50XLS+ Pipet-Lite Multi Pipette L8-200XLS+ Pipet-Lite Multi Pipette L8-10XLS+ Pipet-Lite Multi Pipette L8-20XLS+ Pipet-Lite LTS Pipette L-2XLS+ Pipet-Lite LTS Pipette L-10XLS+ Pipet-Lite LTS Pipette L-20XLS+ Pipet-Lite LTS Pipette L-100XLS+ Pipet-Lite LTS Pipette L-200XLS+ Pipet-Lite LTS Pipette L-1000XLS+	17013804 17013805 17013802 17013803 17014393 17014388 17014392 17014384 17014391 17014382

Additional Kits, Reagents & Equipment

The items in the table below have been validated by 10x Genomics and are highly recommended for the Single Cell V(D)J protocols. Substituting materials may adversely affect system performance.

Supplier	Description	Part Number (US)
Quantification & Quality Control		
Agilent	2100 Bioanalyzer Laptop Bundle	G2943CA
	High Sensitivity DNA Kit	5067-4626
	4200 TapeStation	G2991AA
	High Sensitivity D5000 ScreenTape	5067-5592
	High Sensitivity D5000 Reagents	5067-5593
Choose Bioanalyzer, TapeStation or Qubit based on availability & preference.		
Thermo Fisher Scientific	Qubit 4.0 Fluorometer	Q33226
	Qubit dsDNA HS Assay Kit	Q32854
KAPA Biosystems	KAPA Library Quantification Kit for Illumina Platforms	KK4824

Protocol Steps & Timing

	Steps	Timing	Stop & Store
3 h	Cell Preparation and Labeling Dependent on cell type and labeling protocol used	~1-2 h	
	Step 1 – GEM Generation & Barcoding		
	1.1 Prepare Reaction Mix	20 min	
	1.2 Load Chromium Next GEM Chip G	10 min	
	1.3 Run the Chromium Controller	18 min	
6 h	1.4 Transfer GEMs	3 min	
	1.5 GEM-RT Incubation	55 min	4°C ≤ 72 h or -20°C ≤ 1 week
	Step 2 – Post GEM RT Cleanup		
	2.1 Post GEM-RT Cleanup – Dynabead	45 min	
	Step 3 – cDNA Amplification & QC		
10 h plus*	3.1 cDNA Amplification	50 min	
	3.2 cDNA Cleanup		
	3.2A Pellet Cleanup	15 min	4°C ≤ 72 h or -20°C ≤ 1 week
	3.2B Supernatant Cleanup	20 min	4°C ≤ 72 h or -20°C ≤ 1 week
	3.3 cDNA Quantification & QC	50 min	
	Step 4 – Target Enrichment from cDNA		
	4.1 Target Enrichment 1	40 min	4°C ≤ 72 h
	4.2 Post Target Enrichment 1 Cleanup – SPRIselect	20 min	4°C ≤ 72 h or -20°C ≤ 1 week
	4.3 Target Enrichment 2	40 min	4°C ≤ 72 h
	4.4 Post Target Enrichment 2 Double Sided Size Selection – SPRIselect	30 min	4°C ≤ 72 h or -20°C ≤ 1 week
	4.5 Post Direct Target Enrichment QC & Quantification	50 min	
	Step 5 – Enriched Library Construction		
	5.1 Fragmentation, End Repair & A – tailing	45 min	
	5.2 Adaptor Ligation	25 min	
	5.3 Post Ligation Cleanup – SPRIselect	20 min	
	5.4 Sample Index PCR	40 min	4°C ≤ 72 h
	5.5 Post Sample Index PCR Cleanup – SPRIselect	20 min	4°C ≤ 72 h or -20°C long-term
	5.6 Post Library Construction QC	50 min	
	Step 6 – 5' Gene Expression (GEX) Library Construction		
	6.1 GEX Fragmentation, End Repair & A-tailing	45 min	
	6.2 GEX Post Fragmentation, End Repair & A-tailing Double Sided Size Selection – SPRIselect	30 min	
	6.3 GEX Adaptor Ligation	25 min	
	6.4 GEX Post Ligation Cleanup – SPRIselect	20 min	
	6.5 GEX Sample Index PCR	40 min	4°C ≤ 72 h
	6.6 GEX Post Sample Index PCR Double Sided Cleanup – SPRIselect	30 min	4°C ≤ 72 h or -20°C long-term
	6.7 GEX Post Library Construction QC	50 min	
	Step 7 – Cell Surface Protein Library Construction		
	7.1 Sample Index PCR	30 min	
	7.2 Post Sample Index PCR Size Selection – SPRIselect	20 min	4°C ≤ 72 h or -20°C long-term
	7.3 Post Library Construction QC	50 min	

*Time dependent on Stop options used.

Stepwise Objectives



The Chromium Single Cell V(D)J workflow with Feature Barcoding technology offers a comprehensive, scalable approach to detect cell surface proteins along with the gene expression and immune repertoire information from the same single cell. This is accomplished by labeling cell surface proteins with antibodies conjugated to a Feature Barcode oligonucleotide, followed by direct capture of the Feature Barcode by the Gel Bead primer. To profile the immune repertoire of cells, full-length (5' UTR to constant region), paired T-cell receptor (TCR) and/or B-cell immunoglobulin (Ig) transcripts from 100-10,000 individual cells per sample can be assessed.

A pool of ~750,000 barcodes are sampled separately to index each cell's transcriptome and cell surface protein. It does so by partitioning thousands of cells into nanoliter-scale Gel Beads-in-emulsion (GEMs), where all generated cDNA share a common 10x Barcode. Libraries are generated and sequenced and 10x Barcodes are used to associate individual reads back to the individual partitions.


This document outlines the protocols to generate the following libraries:

- Single Cell V(D)J Enriched libraries from amplified cDNA derived from poly-adenylated mRNA
- Single Cell 5' Gene Expression libraries from amplified cDNA derived from poly-adenylated mRNA
- Single Cell 5' Cell Surface Protein libraries from amplified DNA derived from cell surface protein Feature Barcode

Step 1 GEM Generation & Barcoding

GEMs are generated by combining barcoded Single Cell VDJ 5' Gel Beads v1.1, a Master Mix with cell surface protein labeled cells, and Partitioning Oil onto Chromium Next GEM Chip G.

To achieve single cell resolution, cells are delivered at a limiting dilution, such that the majority (~90 – 99%) of generated GEMs contains no cell, while the remainder largely contain a single cell.

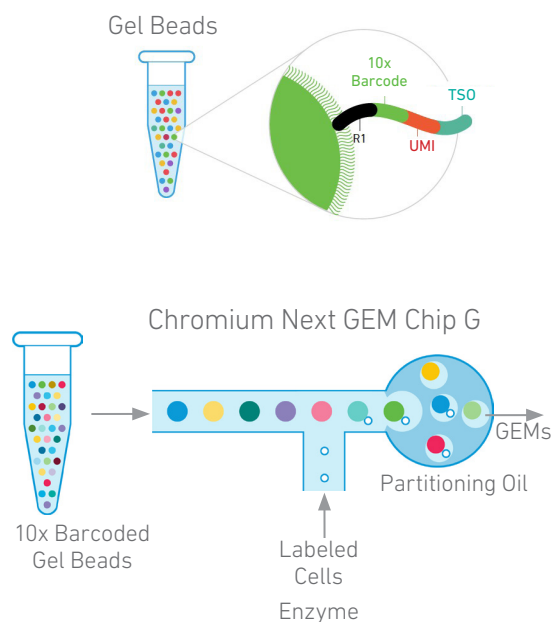


Step 1 GEM Generation & Barcoding

Immediately following GEM generation, the Gel Bead is dissolved and any co-partitioned cell is lysed. Gel Bead primers containing (i) an Illumina TruSeq Read 1 sequence (read 1 sequencing primer), (ii) a 16 nt 10x Barcode, (iii) a 10 nt unique molecular identifier (UMI), and (iv) 13 nt template switch oligo (TSO) are released and mixed with the cell lysate and a Master Mix containing reverse transcription (RT) reagents and poly(dT) primers.

A. The cell lysate and the released Gel Bead primer incubated with the Master Mix containing RT reagents, produce 10x Barcoded, full-length cDNA from poly-adenylated mRNA.

B. Simultaneously in the same partition, the Gel Bead captures the cell surface protein Feature Barcode containing (i) a Nextera Read 2 (Read 2N), (ii) a 15 nt Feature Barcode, and (iii) Capture Sequence. Incubation of the GEMs with the Master Mix containing RT reagents, produces 10x Barcoded, DNA from the cell surface protein Feature Barcode.

Inside individual GEMs

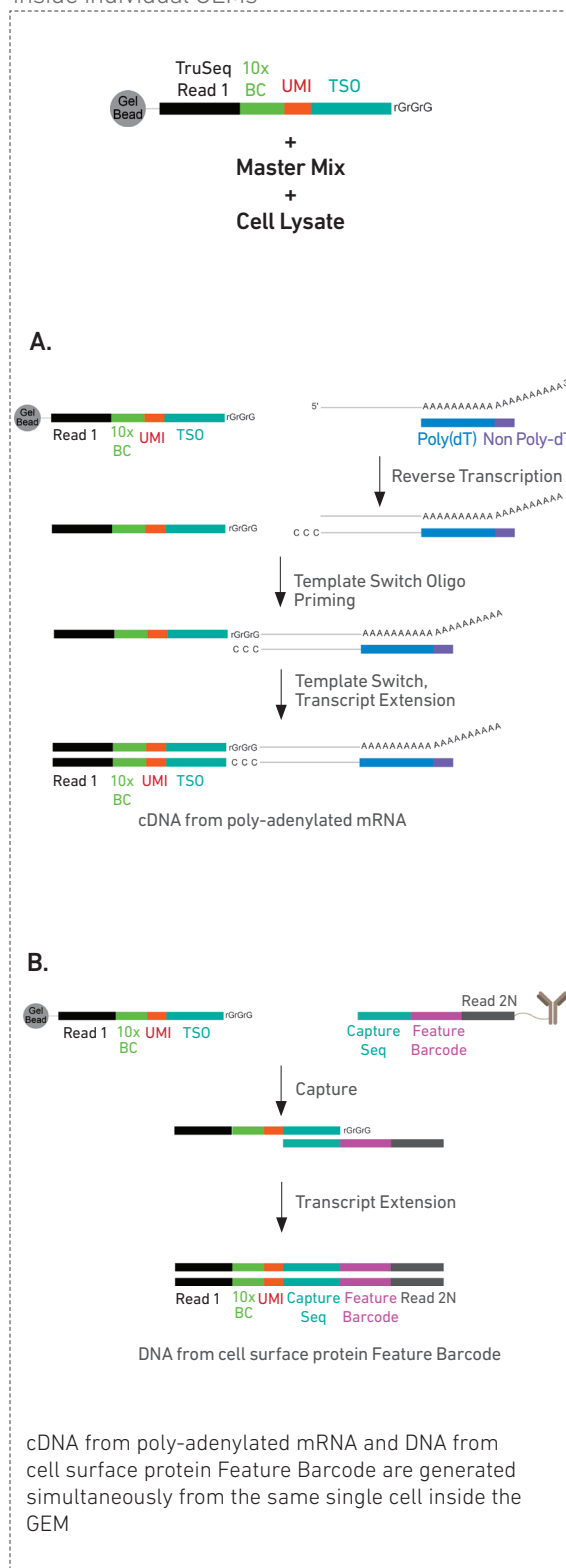

Step 2 Post GEM-RT Cleanup & QC

GEMs are broken and pooled after GEM-RT reaction mixtures are recovered. Silane magnetic beads are used to purify the 10x Barcoded first-strand cDNA from poly-adenylated mRNA and DNA from cell surface protein Feature Barcode from the post GEM-RT reaction mixture, which includes leftover biochemical reagents and primers.


Step 3 cDNA Amplification & QC

10x Barcoded, full-length cDNA from poly-adenylated mRNA and DNA from protein Feature Barcode are amplified. Amplification generates sufficient material to construct multiple libraries from the same cells, e.g. both T and/or B cell Enriched libraries (steps 4 and 5), 5' Gene Expression libraries (step 6), and Cell Surface Protein libraries (step 7).

The amplified cDNA from poly-adenylated mRNA and the amplified DNA from cell surface protein Feature Barcode are separated by size selection for generating V(D)J enriched and 5' Gene Expression libraries and Cell Surface Protein libraries, respectively.

To analyze cell surface protein expression, generate both Cell Surface Protein and 5' Gene Expressions libraries.

Pooled cDNA amplification

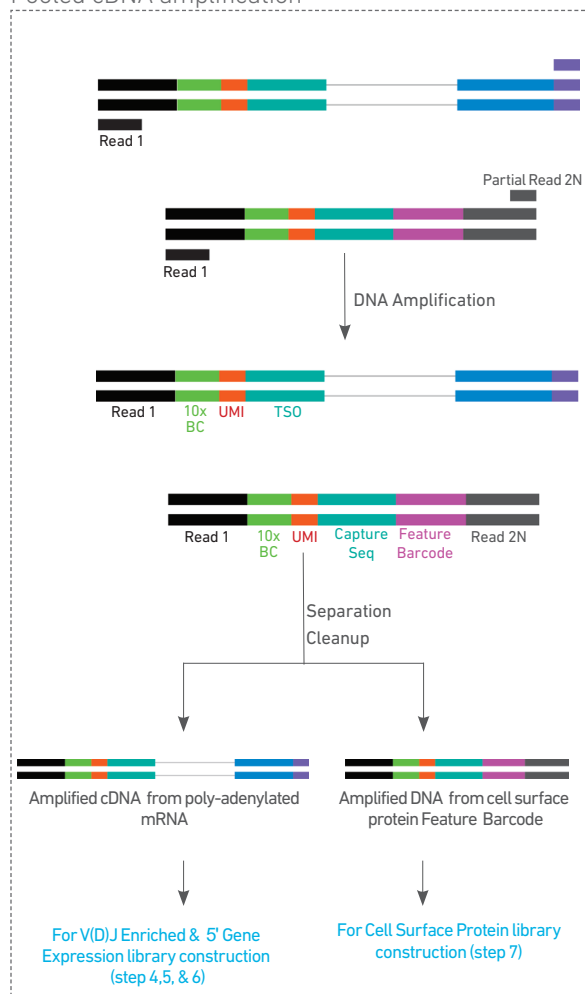

Step 4 Target Enrichment from cDNA


Amplified full-length cDNA from poly-adenylated mRNA is used to enrich full-length V(D)J segments (10x Barcoded) via PCR amplification with primers specific to either the TCR or Ig constant regions. If both T and B cells are expected to be present in the partitioned cell population, TCR and Ig transcripts can be enriched in separate reactions from the same amplified cDNA material. P5 is added during enrichment.

Step 5 Enriched Library Construction

Enzymatic fragmentation and size selection are used to generate variable length fragments that collectively span the V(D)J segments of the enriched TCR or Ig transcripts prior to library construction.

P7, a sample index, and an Illumina R2 sequence (read 2 primer sequence) are added via End Repair, A-tailing, Adaptor Ligation, and Sample Index PCR. The final libraries contain the P5 and P7 priming sites used in Illumina sequencing.


Pooled amplified cDNA processed in bulk

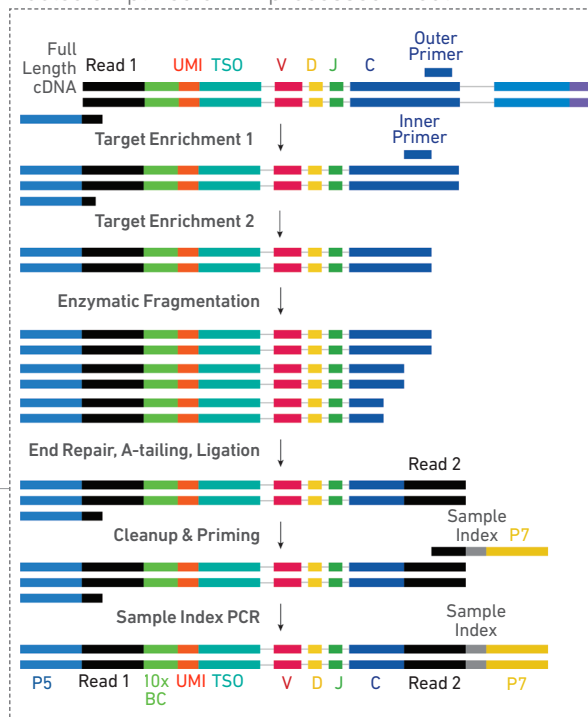

Step 6 5' Gene Expression (GEX) Library Construction

Amplified full-length cDNA from poly-adenylated mRNA is used to generate 5' Gene Expression library. Enzymatic fragmentation and size selection are used to optimize the cDNA amplicon size prior to 5' gene expression library construction. P5, P7, a sample index, and Illumina R2 sequence (read 2 primer sequence) are added via End Repair, A-tailing, Adaptor Ligation, and Sample Index PCR. The final libraries contain the P5 and P7 priming sites used in Illumina sequencers.

Pooled amplified cDNA processed in bulk

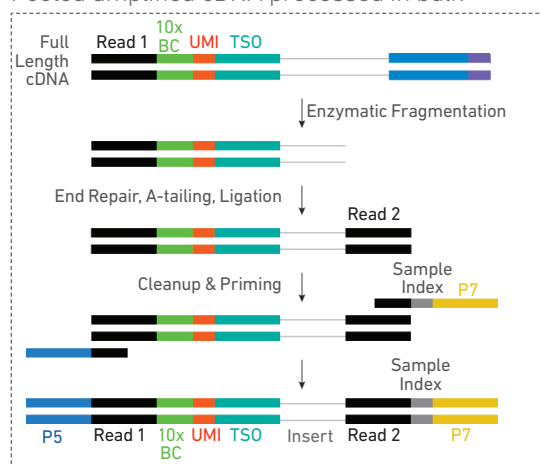


Step 7 Cell Surface Protein Library Construction

Amplified DNA from cell surface protein Feature Barcode is used to construct Cell Surface Protein library. P5, P7, a sample index, and Nextera Read 2 (Read 2N primer sequence) are added via Sample Index PCR.

The final libraries contain the P5 and P7 priming sites used in Illumina sequencers.

To analyze cell surface protein expression, generate both Cell Surface Protein and 5' Gene Expressions libraries.

Pooled amplified DNA processed in bulk

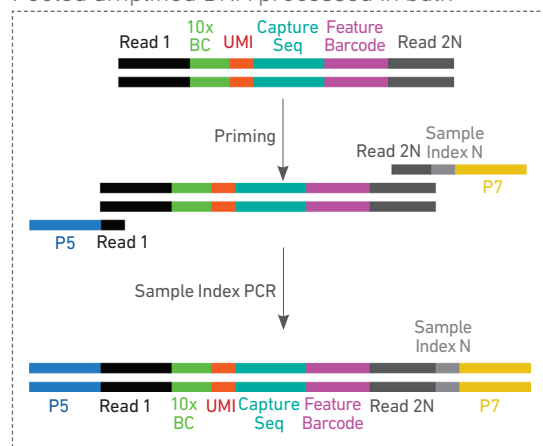

Step 8 Sequencing

Illumina-ready sequencing libraries can be sequenced at the recommended depth & run parameters. Illumina sequencer compatibility, sample indices, library loading and pooling for sequencing are summarized in step 8.


Chromium Single Cell V(D)J Enriched Library



Chromium Single Cell 5' Gene Expression Library



Chromium Single Cell 5' Cell Surface Protein Library

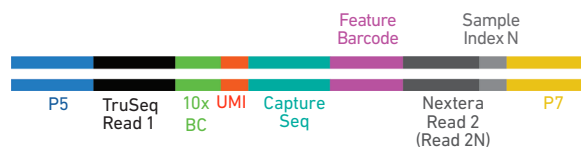


[See Appendix for Oligonucleotide Sequences](#)

Cell Surface Protein Labeling Guidelines

Overview

Cell surface proteins can be labeled using a Feature Barcode oligonucleotide conjugated to a specific protein binding molecule, such as an antibody. Cells can also be labeled using a Feature Barcode oligonucleotide conjugated to a MHC Dextramer, such as a dCODE Dextramer. The Feature Barcode conjugated molecule bound to the cell surface protein can be directly captured by the Gel Bead inside a GEM during GEM generation and amplified (see [Stepwise Objectives](#) for assay scheme specifics). The amplified DNA generated from the Feature Barcode can be used for Cell Surface Protein Library Construction.

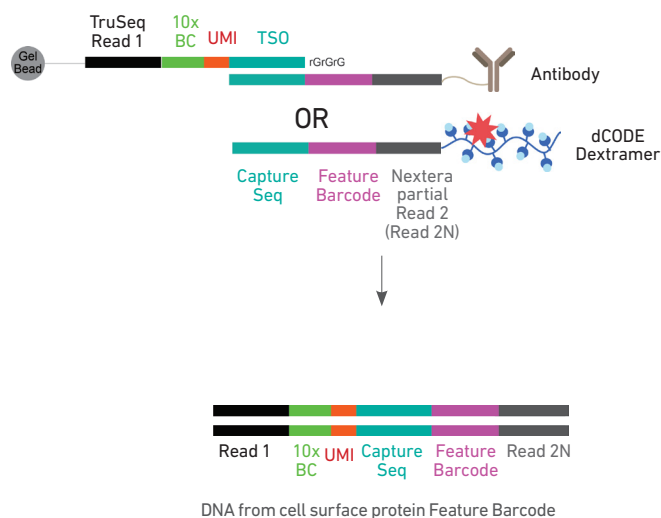

Demonstrated Protocols for cell surface protein labeling

- Demonstrated Protocol Cell Surface Protein Labeling for Single Cell RNA Sequencing Protocols with Feature Barcoding technology (Document CG000149).
- Demonstrated Protocol Cell Labeling with Dextramers for Single Cell RNA Sequencing Protocols with Feature Barcoding technology (Document CG000203).



Failure to label cell surface proteins with a Feature Barcode conjugated to a specific protein binding molecule prior to using the cells for GEM Generation & Barcoding will preclude generation of Cell Surface Protein library.

Tips & Best Practices

TIPS

Icons



Tips & Best Practices section includes additional guidance



Signifies critical step requiring accurate execution



Troubleshooting section includes additional guidance



Next GEM specific protocol step updates

Emulsion-safe Plastics

- Use validated emulsion-safe plastic consumables when handling GEMs as some plastics can destabilize GEMs.

Cell Concentration

- Recommended starting point is to load ~1700 cells per reaction, resulting in recovery of ~1000 cells, and a multiplet rate of ~0.8%. The optimal input cell concentration is 700-1,200 cells/ μ L.
- The presence of dead cells in the suspension may also reduce the recovery rate. Consult the 10x Genomics Single Cell Protocols Cell Preparation Guide and the Guidelines for Optimal Sample Preparation flowchart (Documents CG00053 and CG000126 respectively) for more information on preparing cells.
- Refer to the 10x Genomics Support website for more information regarding cell type specific sample preparation, for example, the Demonstrated Protocol for Enrichment of CD3⁺ T Cells from Dissociated Tissues for Single Cell RNA Sequencing and Immune Repertoire Profiling (Document CG000123).

Multiplet Rate (%)	# of Cells Loaded	# of Cells Recovered
~0.4%	~870	~500
~0.8%	~1,700	~1,000
~1.6%	~3,500	~2,000
~2.3%	~5,300	~3,000
~3.1%	~7,000	~4,000
~3.9%	~8,700	~5,000
~4.6%	~10,500	~6,000
~5.4%	~12,200	~7,000
~6.1%	~14,000	~8,000
~6.9%	~15,700	~9,000
~7.6%	~17,400	~10,000

General Reagent Handling

- Fully thaw and thoroughly mix reagents before use.
- Keep all enzymes and Master Mixes on ice during setup and use. Promptly move reagents back to the recommended storage after use.
- Calculate reagent volumes with 10% excess of 1 reaction values.
- Cover Partitioning Oil tubes and reservoirs to minimize evaporation.
- If using multiple chips, use separate reagent reservoirs for each chip during loading.
- Thoroughly mix samples with the beads during bead-based cleanup steps.

50% Glycerol Solution

- Purchase 50% glycerol solution from Ricca Chemical Company, Glycerin (glycerol), 50% (v/v) Aqueous Solution, PN-3290-32.
- Prepare 50% glycerol solution:
 - i. Mix an equal volume of water and 99% Glycerol, Molecular Biology Grade.
 - ii. Filter through a 0.2- μ m filter.
 - iii. Store at -20°C in 1-ml LoBind tubes. 50% glycerol solution should be equilibrated to room temperature before use.

Pipette Calibration

- Follow manufacturer's calibration and maintenance schedules.
- Pipette accuracy is particularly important when using SPRIselect reagents.

Chromium Next GEM Chip Handling



- Minimize exposure of reagents, chips, and gaskets to sources of particles and fibers, laboratory wipes, frequently opened flip-cap tubes, clothing that sheds fibers, and dusty surfaces.
- After removing the chip from the sealed bag, use in ≤ 24 h.
- Execute steps without pause or delay, unless indicated. When multiple chips are to be used, load, run, and collect the content from one chip before loading the next.
- Fill all unused input wells in rows labeled 1, 2, and 3 on a chip with an appropriate volume of 50% glycerol solution before loading the used wells. **DO NOT** add glycerol to the wells in the bottom NO FILL row.
- Avoid contacting the bottom surface of the chip with gloved hands and other surfaces. Frictional charging can lead to inadequate priming of the channels, potentially leading to either clogs or wetting failures.
- Minimize the distance that a loaded chip is moved to reach the Chromium Controller.
- Keep the chip horizontal to prevent wetting the gasket with oil, which depletes the input volume and may adversely affect the quality of the resulting emulsion.

Chromium Next GEM Secondary Holders



- Chromium Next GEM Secondary Holders encase Chromium Next GEM Chips.
- The holder lid flips over to become a stand, holding the chip at 45 degrees for optimal recovery well content removal.
- Squeeze the black sliders on the back side of the holder together to unlock the lid and return the holder to a flat position.



Chromium Next GEM Chip & Holder Assembly



- Align notch on the chip (upper left corner) and the holder.
- Insert the left-hand side of the chip under the guide. Depress the right-hand side of the chip until the spring-loaded clip engages.
- Close the lid before dispensing reagents into the wells.



Chromium Next GEM Chip Loading




- Place the assembled chip and holder flat on the bench with the lid closed.
- Dispense at the bottom of the wells without introducing bubbles.
- When dispensing Gel Beads into the chip, wait for the remainder to drain into the bottom of the pipette tips and dispense again to ensure complete transfer.
- Refer to [Load Chromium Next GEM Chip G](#) for specific instructions.



Gel Bead Handling



- Use one tube of Gel Beads per sample. **DO NOT** puncture the foil seals of tubes not used at the time.
- Equilibrate the Gel Beads strip to room temperature before use.
- Store unused Gel Beads at -80°C and avoid more than 12 freeze-thaw cycles. **DO NOT** store Gel Beads at -20°C .
- Snap the tube strip holder with the Gel Bead strip into a 10x Vortex Adapter. Vortex **30 sec**.
- Centrifuge the Gel Bead strip for **~5 sec** after removing from the holder. Confirm there are no bubbles at the bottom of the tubes and the liquid levels look even. Place the Gel Bead strip back in the holder and secure the holder lid.
- If the required volume of beads cannot be recovered, place the pipette tips against the sidewalls and slowly dispense the Gel Beads back into the tubes. **DO NOT** introduce bubbles into the tubes and verify that the pipette tips contain no leftover Gel Beads. Withdraw the full volume of beads again by pipetting slowly.

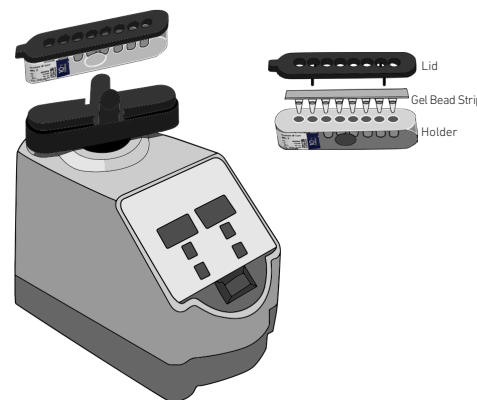

10x Gasket Attachment

- After reagents are loaded, attach the gasket by holding the tongue (curved end, to the right) and hook it on the left-hand tabs of the holder. Gently pull the gasket toward the right and hook it on the two right-hand tabs.
- DO NOT touch the smooth side of the gasket. DO NOT press down on the top of the gasket after attachment.
- Keep the assembly horizontal to avoid wetting the gasket with Partitioning Oil.




10x Magnetic Separator

- Offers two positions of the magnets (high and low) relative to a tube, depending on its orientation. Flip the magnetic separator over to switch between high (magnet•**High**) or low (magnet•**Low**) positions.
- If using MicroAmp 8-Tube Strips, use the high position (magnet•**High**) only throughout the protocol.



Magnetic Bead Cleanup Steps

- During magnetic bead based cleanup steps that specify waiting “until the solution clears”, visually confirm clearing of solution before proceeding to the next step. See adjacent panel for an example.
- The time need for the solution to clear may vary based on specific step, reagents, volume of reagents used etc.

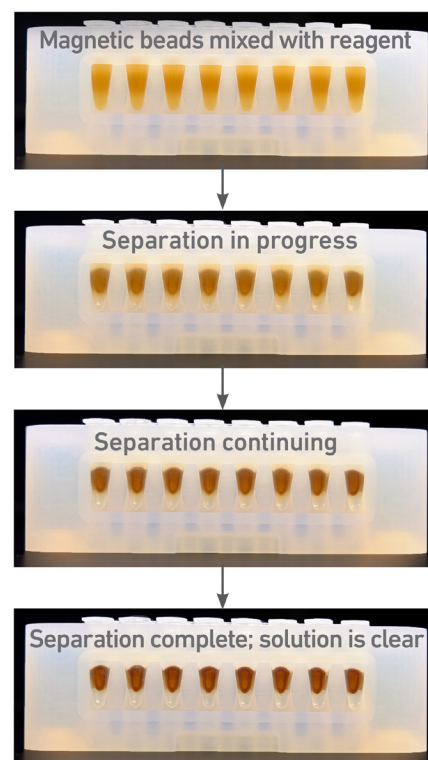

cDNA Amplification PCR Cycle Numbers

- Follow cycle number recommendations for high and low RNA content cells based on Targeted Cell Recovery and cell sample.
- Cycle numbers in the table below have been optimized assuming that the sample has >80% T and/or B cells. Samples with lower fraction of T and/or B cells may require additional cycle number optimization and/or may be enriched to increase the fraction of T or B cells. Refer to the Demonstrated Protocol for Enrichment of CD3+ T Cells from Dissociated Tissues for Single Cell RNA Sequencing and Immune Repertoire Profiling (Document CG000123).
- If the fraction of T and/or B cells in a cell sample is known, adjust PCR cycle number based on that fraction to ensure sufficient product generation.

Tutorial – Optimizing cDNA Amplification PCR Cycle Numbers

Examples

Sample A:

Primary cells with 15% T cell fraction.
Targeted Cell Recovery is 10,000 cells.
Only 1,500 (15%) cells are T cells.
Total PCR cycles – 16.

Recommended starting point for cycle number optimization.

Sample B:

Cell line with high RNA content.
Targeted Cell Recovery is 10,000 cells.
Total PCR cycles – 11.

Sample C:

Cell mix with 90% low RNA content and 10% high RNA content B cells.
Targeted Cell Recovery is 10,000 cells.
90% B cells are low RNA content.
Total PCR cycles – 13.

Targeted Cell Recovery	Low RNA Content Cells Total Cycles	High RNA Content Cells Total Cycles
100-500	18	16
501-2,000	16	14
2,001-6,000	14	12
6,001-10,000	13	11

Enzymatic Fragmentation

- Ensure enzymatic fragmentation reactions are prepared on ice and then loaded into a thermal cycler pre-cooled to 4°C prior to initiating the Fragmentation, End Repair, and A-tailing incubation steps.

SPRIselect Cleanup & Size Selection


- After aspirating the desired volume of SPRIselect reagent, examine the pipette tips before dispensing to ensure the correct volume is transferred.
- Pipette mix thoroughly as insufficient mixing of sample and SPRIselect reagent will lead to inconsistent results.
- Use fresh preparations of 80% Ethanol.

Tutorial — SPRIselect Reagent : DNA Sample Ratios

SPRI beads selectively bind DNA according to the ratio of SPRIselect reagent (beads).

Example: Ratio = $\frac{\text{Volume of SPRIselect reagent added to the sample}}{\text{Volume of DNA sample}} = \frac{50 \mu\text{l}}{100 \mu\text{l}} = 0.5X$

Schematic of Double Sided Size Selection

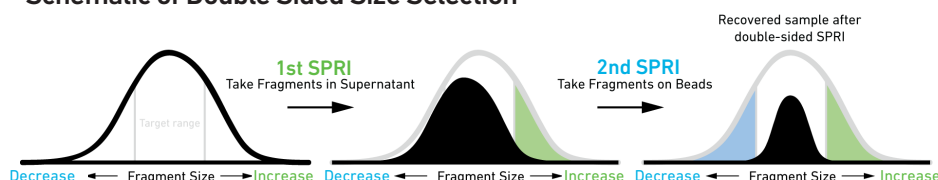

After the first SPRI, supernatant is transferred for a second SPRI while larger fragments are discarded (green). After the second SPRI, fragments on beads are eluted and kept while smaller fragments are discarded (blue). Final sample has a tight fragment size distribution with reduced overall amount (black).

Tutorial — Double Sided Size Selection

Step a – First SPRIselect: Add 50 μl SPRIselect reagent to 100 μl sample (0.5X).

Ratio = $\frac{\text{Volume of SPRIselect reagent added to the sample}}{\text{Volume of DNA sample}} = \frac{50 \mu\text{l}}{100 \mu\text{l}} = 0.5X$

Step b – Second SPRIselect: Add 30 μl SPRIselect reagent to supernatant from step a (0.8X).

Ratio = $\frac{\text{Total Volume of SPRIselect reagent added to the sample (step a + b)}}{\text{Original Volume of DNA sample}} = \frac{50 \mu\text{l} + 30 \mu\text{l}}{100 \mu\text{l}} = 0.8X$

Sample Indices in Sample Index PCR

- Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run.
- Each well in the i7 Sample Index plate contains a unique mix of 4 oligos. The sample indices can therefore be used in any combination.
- Each sample index set is base-balanced to avoid monochromatic signal issues when it is the sole sample loaded on an Illumina sequencer.
- For V(D)J Enriched and 5' Gene Expression libraries, use **ONLY** Chromium i7 Sample Index Plate
- For Cell Surface Protein library, use **ONLY** Chromium i7 Sample Index Plate N, Set A
- Consider sample index compatibility when pooling different libraries; unique sample index for each of the pooled libraries is required.
- The sample indices of Chromium i7 Sample Index Plate are unique from those of Chromium i7 Sample Index Plate N Set A. Therefore, respective libraries from the two plates may be pooled.

Step 1

GEM Generation & Barcoding

- 1.1 Prepare Master Mix
- 1.2 Load Chromium Next GEM Chip G
- 1.3 Run the Chromium Controller
- 1.4 Transfer GEMs
- 1.5 GEM-RT Incubation

1

1.0 GEM Generation & Barcoding



GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	Single Cell VDJ 5' Gel Beads v1.1	2000209	Equilibrate to room temperature 30 min before loading the chip.	-80°C
	● RT Reagent B	2000165	Vortex, verify no precipitate, centrifuge briefly.	-20°C
	● Poly-dT RT Primer	2000007	Vortex, verify no precipitate, centrifuge briefly.	-20°C
	● Additive A	220074	Vortex, verify no precipitate, centrifuge briefly.	-20°C
Place on Ice	○ RT Enzyme Mix B	2000010/ 2000021	Centrifuge briefly before adding to the mix.	-20°C
<div> Labeled Cells Refer to Demonstrated Protocols for Cell Surface Protein Labeling (CG000149, CG000203). </div>				
Obtain	Partitioning Oil	2000190	-	Ambient
	Chromium Next GEM Chip G	2000177	-	Ambient
	10x Gasket	370017/ 3000072	See Tips & Best Practices.	Ambient
	Chromium Next GEM Secondary Holder	3000332	See Tips & Best Practices.	Ambient
	10x Vortex Adapter	330002	See Tips & Best Practices.	Ambient
	50% glycerol solution If using <8 reactions	-	See Tips & Best Practices.	-



Firmware Version 4.0 or higher is required in the Chromium Controller or the Chromium Single Cell Controller used for the Single Cell V(D)J v1.1 protocol.

1.1 Prepare Reaction Mix

Next
GEM

a. Prepare Master Mix on ice. Pipette mix 15x and centrifuge briefly.

Master Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
● RT Reagent B	2000165	18.8	82.5	165.0
● Poly-dT RT Primer	2000007	6.4	28.1	56.2
● Additive A	220074	2.0	8.8	17.6
○ RT Enzyme Mix B	2000010/ 2000021	10.0	44.0	88.0
Total	-	37.2	163.4	326.8

b. Add 37.2 μl Master Mix into each tube of a PCR 8-tube strip on ice.

Assemble Chromium Next GEM Chip G




After removing the chip from the sealed bag, use the chip in ≤ 24 h.



See Tips & Best Practices for chip handling instructions.

- Align notch on the chip (upper left corner) and the holder.
- Insert the left-hand side of the chip under the guide. Depress the right-hand side of the chip until the spring-loaded clip engages.
- Close the lid before dispensing reagents into the wells.
- The assembled chip is ready for loading the indicated reagents. Refer to step 1.2 for reagent volumes and loading order.

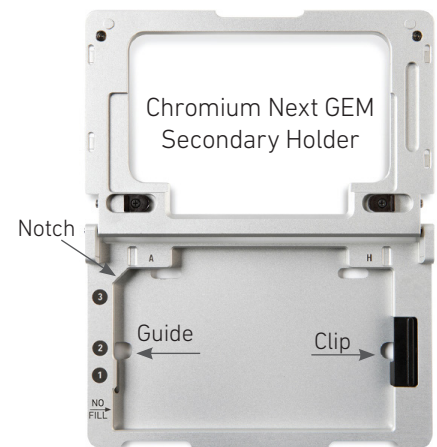

For GEM generation, load the indicated reagents only in the specified rows, starting from row labeled 1, followed by rows labeled 2 and 3. DO NOT load reagents in the bottom row labeled NO FILL. See step 1.2 for details.





Cell Suspension Volume Calculator Table

(for step 1.2 of Chromium Next GEM Single Cell V(D)J v1.1 protocol)

Volume of Labeled Cell Suspension Stock per reaction (µl) | Volume of Nuclease-free Water per reaction (µl)

Cell Stock Concentration (Cells/µl)	Targeted Cell Recovery										
	500	1000	2000	3000	4000	5000	6000	7000	8000	9000	10000
100	8.3	16.5	33.0	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a
	29.5	21.3	4.8								
200	4.1	8.3	16.5	24.8	33.0	n/a	n/a	n/a	n/a	n/a	n/a
	33.7	29.5	21.3	13.0	4.8						
300	2.8	5.5	11.0	16.5	22.0	n/a	n/a	n/a	n/a	n/a	n/a
	35.0	32.3	26.8	21.3	15.8						
400	2.1	4.1	8.3	12.4	16.5	20.6	24.8	28.9	33.0	n/a	n/a
	35.7	33.7	29.5	25.4	21.3	17.2	13.0	8.9	4.8		
500	1.7	3.3	6.6	9.9	13.2	16.5	19.8	23.1	26.4	29.7	33.0
	36.1	34.5	31.2	27.9	24.6	21.3	18.0	14.7	11.4	8.1	4.8
600	1.5	2.8	5.5	8.3	11.0	13.8	16.5	19.3	22.0	24.8	27.5
	36.3	35.0	32.3	29.5	26.8	24.0	21.3	18.5	15.8	13.0	10.3
700	1.2	2.4	4.7	7.1	9.4	11.8	14.1	16.5	18.9	21.2	23.6
	36.6	35.4	33.1	30.7	28.4	26.0	23.7	21.3	18.9	16.6	14.2
800	1.0	2.1	4.1	6.2	8.3	10.3	12.4	14.4	16.5	18.6	20.6
	36.8	35.7	33.7	31.6	29.5	27.5	25.4	23.4	21.3	19.2	17.2
900	0.9	1.8	3.7	5.5	7.3	9.2	11.0	12.8	14.7	16.5	18.3
	36.9	36.0	34.1	32.3	30.5	28.6	26.8	25.0	23.1	21.3	19.5
1000	0.8	1.7	3.3	5.0	6.6	8.3	9.9	11.6	13.2	14.8	16.5
	37.0	36.1	34.5	32.8	31.2	29.5	27.9	26.2	24.6	23.0	21.3
1100	0.8	1.5	3.0	4.5	6.0	7.5	9.0	10.5	12.0	13.5	15.0
	37.0	36.3	34.8	33.3	31.8	30.3	28.8	27.3	25.8	24.3	22.8
1200	0.7	1.4	2.8	4.1	5.5	6.9	8.3	9.6	11.0	12.4	13.8
	37.1	36.4	35.0	33.7	32.3	30.9	29.5	28.2	26.8	25.4	24.0
1300	0.6	1.3	2.5	3.8	5.1	6.3	7.6	8.9	10.2	11.4	12.7
	37.2	36.5	35.3	34.0	32.7	31.5	30.2	28.9	27.6	26.4	25.1
1400	0.6	1.2	2.4	3.5	4.7	5.9	7.1	8.3	9.4	10.6	11.8
	37.2	36.6	35.4	34.3	33.1	31.9	30.7	29.5	28.4	27.2	26.0
1500	0.5	1.1	2.2	3.3	4.4	5.5	6.6	7.7	8.8	9.9	11.0
	37.3	36.7	35.6	34.5	33.4	32.3	31.2	30.1	29.0	27.9	26.8
1600	0.5	1.0	2.1	3.1	4.1	5.2	6.2	7.2	8.3	9.3	10.3
	37.3	36.8	35.7	34.7	33.7	32.6	31.6	30.6	29.5	28.5	27.5
1700	0.5	1.0	1.9	2.9	3.9	4.9	5.8	6.8	7.8	8.7	9.7
	37.3	36.8	35.9	34.9	33.9	32.9	32.0	31.0	30.0	29.1	28.1
1800	0.5	0.9	1.8	2.8	3.7	4.6	5.5	6.4	7.3	8.3	9.2
	37.3	36.9	36.0	35.0	34.1	33.2	32.3	31.4	30.5	29.5	28.6
1900	0.4	0.9	1.7	2.6	3.5	4.3	5.2	6.1	6.9	7.8	8.7
	37.4	36.9	36.1	35.2	34.3	33.5	32.6	31.7	30.9	30.0	29.1
2000	0.4	0.8	1.7	2.5	3.3	4.1	5.0	5.8	6.6	7.4	8.3
	37.4	37.0	36.1	35.3	34.5	33.7	32.8	32.0	31.2	30.4	29.5

Grey boxes:

Volumes that would exceed the allowable water volume in each reaction

Yellow boxes:

Indicate a low transfer volume that may result in higher cell load variability

Blue boxes:

Optimal range of cell stock concentration to maximize the likelihood of achieving the desired cell recovery target

1.2 Load Chromium Next GEM Chip G

Next
GEM

! After removing the chip from the sealed bag, use in ≤ 24 h. For all **chip loading steps**, raising and depressing the pipette plunger should each take **~5 sec**. When dispensing, raise the pipette tips at the same rate as the liquid is rising, keeping the tips slightly submerged.

a. Dispense 50% Glycerol into Unused Chip Wells (if < 8 samples per chip)

- 70 μ l to unused wells in row labeled 1.
 - 50 μ l to unused wells in row labeled 2.
 - 45 μ l to unused wells in row labeled 3.
- DO NOT add 50% glycerol solution to the bottom row of NO FILL wells. DO NOT use any substitute for 50% glycerol solution.

b. Prepare Master Mix + Cell Suspension

Refer to the Cell Suspension Volume Calculator Table. Add the appropriate volume of **nuclease-free water** and corresponding volume of **single cell suspension** to Master Mix for a total of 75 μ l in each tube. Gently pipette mix the cells suspension before adding to the Master Mix.


c. Load Row Labeled 1

Gently pipette mix the Master Mix + Cell Suspension and using the same pipette tip, dispense 70 μ l Master Mix + Cell Suspension into the bottom center of each well in **row labeled 1** without introducing bubbles.



d. Prepare Gel Beads

Snap the tube strip holder with the Gel Bead strip into a 10x Vortex Adapter. Vortex 30 sec. Centrifuge the Gel Bead strip for ~5 sec. Confirm there are no bubbles at the bottom of the tubes and the liquid levels are even. Place the Gel Bead strip back in the holder. Secure the holder lid.

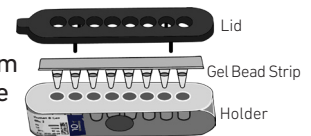

e. Load Row Labeled 2

Puncture the foil seal of the Gel Bead tubes. Slowly aspirate 50 μ l Gel Beads. Dispense into the wells in **row labeled 2** without introducing bubbles. Wait 30 sec.



f. Load Row Labeled 3


Dispense 45 μ l Partitioning Oil into the wells in **row labeled 3** from a reagent reservoir. Failure to add Partitioning Oil to the top row labeled 3 will prevent GEM generation and can damage the Chromium Controller.



! Attach the gasket and run the chip in the Chromium Controller **immediately** after loading the Partitioning Oil.

g. Attach 10x Gasket

Align the notch with the top left-hand corner. Ensure the gasket holes are aligned with the wells. Avoid touching the smooth surface.

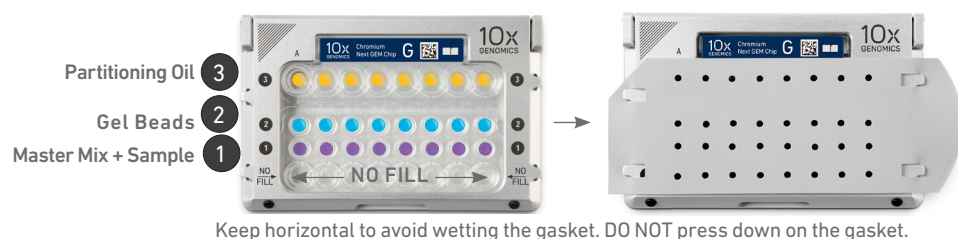

1.3 Run the Chromium Controller

Next
GEM

- Press the eject button on the Controller to eject the tray.
- Place the assembled chip with the gasket in the tray, ensuring that the chip stays horizontal. Press the button to retract the tray.
- Confirm the Chromium Chip G program on screen. Press the play button.
- At completion of the run (~18 min), the Controller will chime. **Immediately** proceed to the next step.



Firmware Version 4.0 or higher is required in the Chromium Controller or the Chromium Single Cell Controller used for the Single Cell V(D)J v1.1 protocol.



1.4 Transfer GEMs

Next
GEM

- Place a tube strip on ice.
- Press the eject button of the Controller and remove the chip.
- Discard the gasket. Open the chip holder. Fold the lid back until it clicks to expose the wells at 45 degrees.
- Check the volume in rows labeled 1-2. Abnormally high volume in any well indicates a clog.
- Slowly aspirate **100 μ l** GEMs from the lowest points of the recovery wells in the top row labeled 3 without creating a seal between the pipette tips and the bottom of the wells.
- Withdraw pipette tips from the wells. GEMs should appear opaque and uniform across all channels. Excess Partitioning Oil (clear) in the pipette tips indicates a potential clog.
- Over the course of **~20 sec**, dispense GEMs into the tube strip on ice with the pipette tips against the sidewalls of the tubes.
- If multiple chips are run back-to-back, cap/cover the GEM-containing tube strip and place on ice for no more than **1 h**.




Expose Wells at 45 Degrees



Transfer GEMs



GEMs

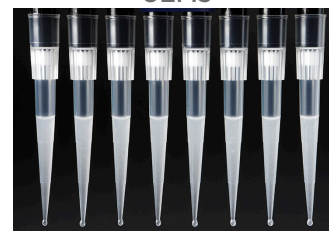

1.5
GEM-RT Incubation

Use a thermal cycler that can accommodate at least 100 µl volume. A volume of 125 µl is the preferred setting on Bio-Rad C1000 Touch. In alternate thermal cyclers, use highest reaction volume setting.

a. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
53°C	125 µl	~55 min

Step	Temperature	Time
1	53°C	00:45:00
2	85°C	00:05:00
3	4°C	Hold



b. Store at 4°C for up to 72 h or at –20°C for up to a week, or proceed to the next step.

Step 2

Post GEM-RT Cleanup

2.1 Post GEM-RT Cleanup – Dynabeads

2.0

Post GEM-RT Cleanup

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	● Additive A	220074	Thaw, vortex, verify no precipitate, centrifuge briefly.	-20°C
	Dynabeads MyOne SILANE	2000048	Vortex thoroughly (≥30 sec) immediately before adding to the mix. If still clumpy, pipette mix to resuspend completely. DO NOT centrifuge before use.	4°C
Thaw at 65°C	● Buffer Sample Clean Up 1	220020	Thaw for 10 min at 65°C at max speed on a thermomixer. Verify there are no visible crystals. Cool to room temperature.	-20°C
Obtain	○ Recovery Agent	220016	-	Ambient
	Qiagen Buffer EB	-	Manufacturer's recommendations.	-
	Bio-Rad 10% Tween 20	-	Manufacturer's recommendations.	-
	10x Magnetic Separator	230003	-	Ambient
	Prepare 80% Ethanol Prepare 15 ml for 8 reactions.	-	Prepare fresh.	-

2.1 Post GEM-RT Cleanup – Dynabeads

- a. Add **125 µl** Recovery Agent to each sample (post GEM-RT incubation) at room temperature. **DO NOT** pipette mix or vortex the biphasic mixture. Wait **2 min**.

The resulting biphasic mixture contains Recovery Agent/Partitioning Oil (pink) and aqueous phase (clear), with no persisting emulsion (opaque).

If biphasic separation is incomplete:

Firmly secure the cap on the tube strip, ensuring that no liquid is trapped between the cap and the tube rim. Mix by inverting the capped tube strip 5x, centrifuge briefly, and proceed to step b. **DO NOT** invert without firmly securing the caps.

Biphasic Mixture




A smaller aqueous phase volume indicates a clog during GEM generation.





- b. Slowly remove and discard **125 µl** Recovery Agent/Partitioning Oil (pink) from the bottom of the tube. **DO NOT** aspirate any aqueous sample.

Remove Recovery Agent

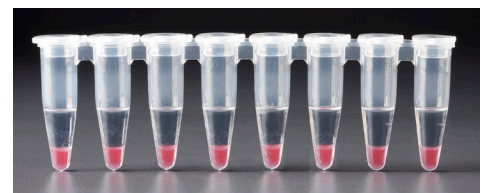

- c. Prepare Dynabeads Cleanup Mix.


Dynabeads Cleanup Mix <i>Add reagents in the order listed</i>	PN	1X (µl)	4X + 10% (µl)	8X + 10% (µl)
Nuclease-free Water		5	22	44
● Buffer Sample Clean Up 1	220020	182	801	1602
Dynabeads MyOne SILANE Vortex thoroughly (≥30 sec) immediately before adding to the mix.				
  Aspirate the full liquid volume with a pipette tip to verify that the beads have not settled in the bottom of the tube. If clumps are present, pipette mix to resuspend completely. DO NOT centrifuge before use.	2000048	8	35	70
● Additive A	220074	5	22	44
Total	-	200	880	1760

Add Dynabeads Cleanup Mix



- d. Vortex and add **200 µl** to each sample. Pipette mix 5x (pipette set to 200 µl).
- e. Incubate **10 min** at room temperature.

f. Prepare Elution Solution I. Vortex and centrifuge briefly.

Elution Solution I <i>Add reagents in the order listed</i>	PN	1X (μl)	10X (μl)
Buffer EB	-	98	980
10% Tween 20	-	1	10
 Additive A	220074	1	10
Total	-	100	1000

g. At the end of **10 min** incubation, place on a 10x Magnetic Separator • **High position** (magnet • **High**) until the solution clears.

A white interface between the aqueous phase and Recovery Agent is normal.

h. Remove the supernatant.

i. Add **300 μl** 80% ethanol to the pellet while on the magnet. Wait **30 sec**.

j. Remove the ethanol.

k. Add **200 μl** 80% ethanol to pellet. Wait **30 sec**.

l. Remove the ethanol.

m. Centrifuge briefly. Place on the magnet • **Low**.n. Remove remaining ethanol. Air dry for **2 min**.o. Remove from the magnet. Immediately add **35.5 μl** Elution Solution I.

p. Pipette mix (pipette set to 30 μl) without introducing bubbles. Pipette mix 15x. If beads still appear clumpy, continue pipette mixing until fully resuspended.




q. Incubate **1 min** at **room temperature**.r. Place on the magnet • **Low** until the solution clears.s. Transfer **35 μl** sample to a new tube strip.

Step 3

cDNA Amplification & QC




- 3.1 cDNA Amplification
- 3.2 cDNA Cleanup – SPRIselect
- 3.3 cDNA QC & Quantification

3.0 cDNA Amplification & QC

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	 SC5' Feature cDNA Primers  Verify name & PN	2000119	Vortex, centrifuge briefly.	-20°C
	Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
	Agilent Bioanalyzer High Sensitivity Kit If used for QC and quantification	-	Manufacturer's recommendations.	-
	Agilent TapeStation ScreenTape and Reagents If used for QC and quantification	-	Manufacturer's recommendations.	-
	Qubit dsDNA HS Assay Kit If used for quantification	-	Manufacturer's recommendations.	-
Place on ice	 Amplification Master Mix	220125	Vortex, centrifuge briefly.	-20°C
Obtain	Qiagen Buffer EB	-	Manufacturer's recommendations.	-
	10x Magnetic Separator	230003	-	Ambient
	Prepare 80% Ethanol Prepare 15 ml for 8 samples	-	Prepare fresh.	-

3.1 cDNA Amplification

a. Prepare cDNA Amplification Mix on ice. Vortex and centrifuge briefly.

cDNA Amplification Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
 Amplification Master Mix	220125	50	220	440
 SC5' Feature cDNA Primers	2000119	15	66	132
 Verify name & PN				
Total	-	65	286	572

b. Add **65 μl** cDNA Amplification Mix to **35 μl** sample (Post GEM-RT Cleanup, step 2.1s).

c. Pipette mix 5x (pipette set to 90 μl). Centrifuge briefly.

d. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~25-50 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	67°C	00:00:30
4	72°C	00:01:00
5	Go to Step 2, see table below for total # of cycles	
6	72°C	00:01:00
7	4°C	Hold

Recommended starting point for cycle number optimization.





The optimal number of cycles is a trade-off between generating sufficient final mass for library construction and minimizing PCR amplification artifacts. Cycle numbers were optimized assuming that sample includes >80% T or B cells. If testing cells types with a known fraction of T and/or B cells, adjust cycle number based on that fraction to generate sufficient product. See Tips and Best Practices for examples.

Targeted Cell Recovery	Primary Cells Total Cycles	Cell Lines Total Cycles
100 -500	18	16
501-2,000	16	14
2,001-6,000	14	12
6,001-10,000	13	11




e. Store at **4°C** for up to **72 h** or proceed to the next step.

Step Overview
(steps 3.1 & 3.2)

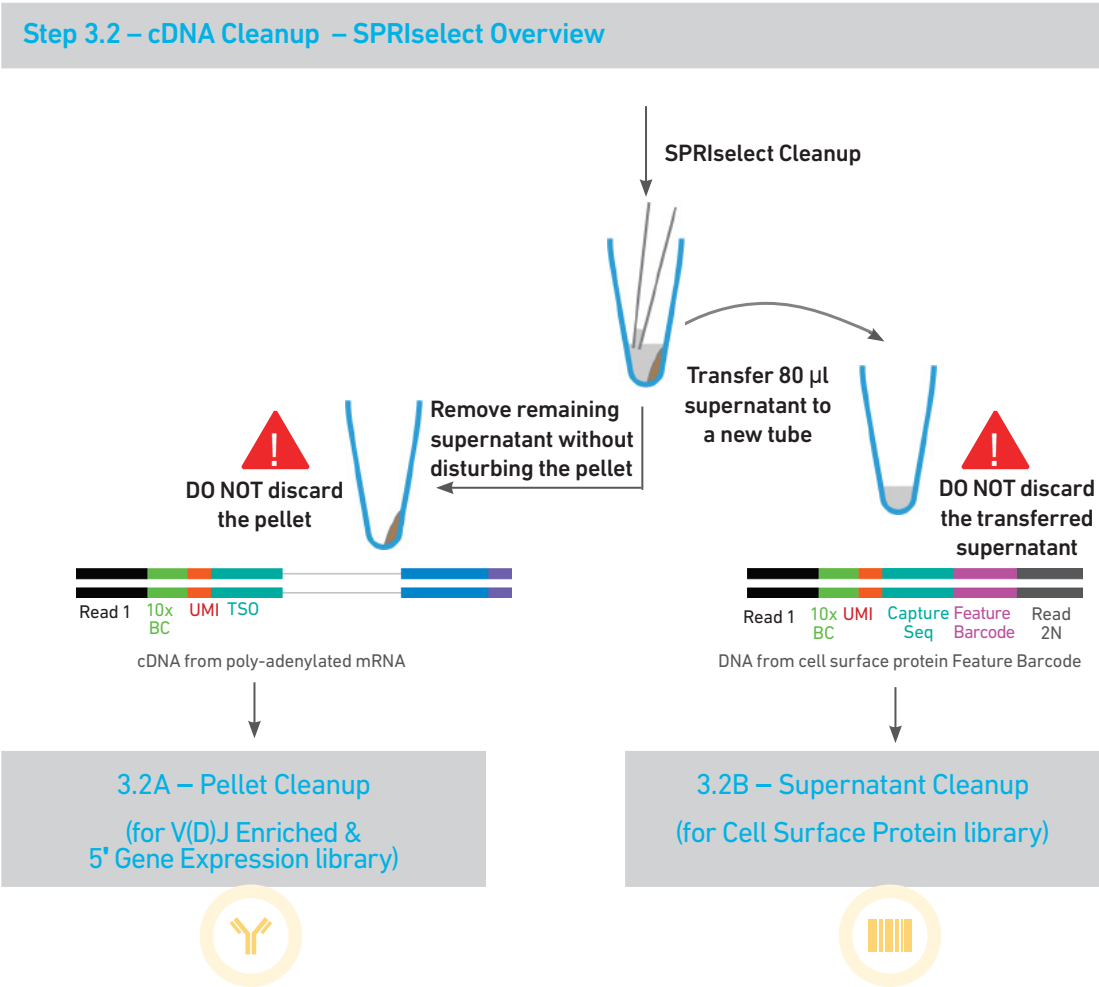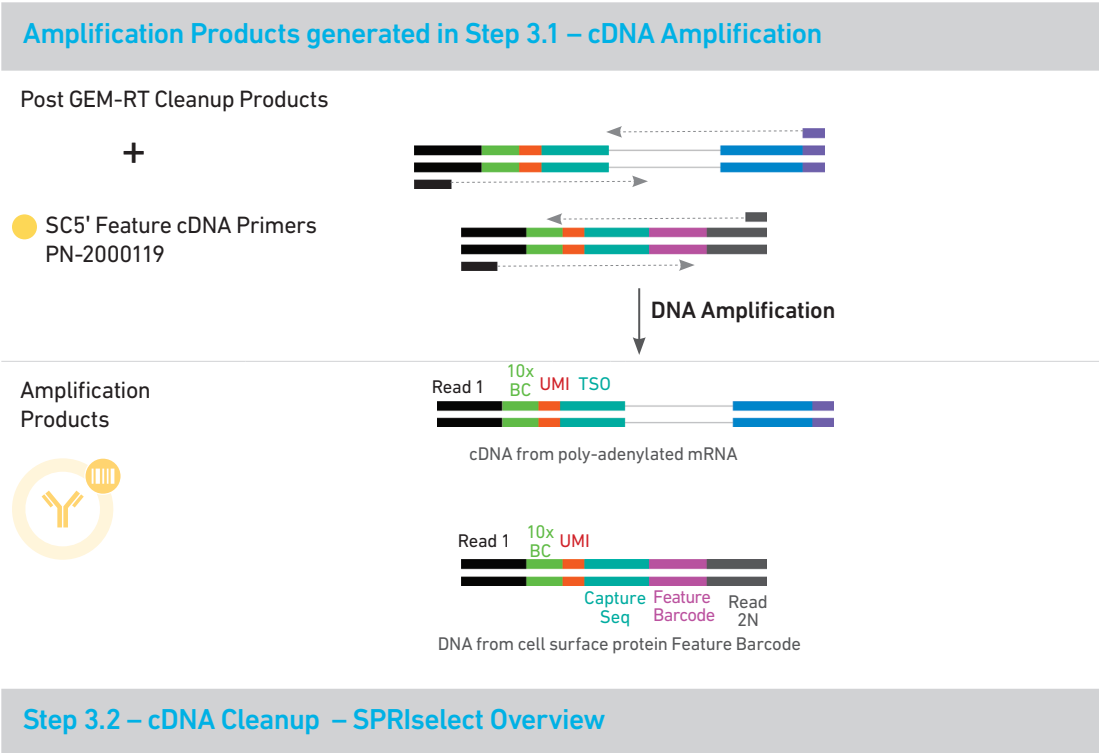


3.2 cDNA Cleanup – SPRIselect

- a. Vortex to resuspend the SPRIselect reagent. Add **60 µl** SPRIselect reagent (**0.6X**) to each sample and pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears.
- d.  Transfer and save **80 µl** supernatant in a new tube strip without disturbing the pellet. Maintain at **room temperature**. DO NOT discard the transferred supernatant (cleanup for Cell Surface Protein library construction).
- e. Remove the remaining supernatant from the pellet without disturbing the pellet. DO NOT discard the pellet (cleanup for Enriched and 5' Gene Expression library construction). **Immediately** proceed to Pellet Cleanup (step 3.2A).


3.2A Pellet Cleanup

(for V(D)J Enriched & 5' Gene Expression library)

- i. Add **200 µl** 80% ethanol to the pellet while still on magnet•**High**. Wait **30 sec**.
- ii. Remove the ethanol.
- iii. **Repeat** steps i and ii for a total of 2 washes.
- iv. Centrifuge briefly and place on the magnet•**Low**.
- v. Remove any remaining ethanol. Air dry for **2 min**. DO NOT exceed **2 min** as this will decrease elution efficiency.
- vi. Remove from the magnet. Add **45.5 µl** Buffer EB. Pipette mix 15x.
- vii. Incubate **2 min** at **room temperature**.
- viii. Place the tube strip on the magnet•**High** until the solution clears.
- ix. Transfer **45 µl** sample to a new tube strip.
- x.  Store at **4°C** for up to **72 h** or at **–20°C** for up to a **week**, or proceed to **step 3.3 for cDNA QC & Quantification**.

3.2B Transferred Supernatant Cleanup

(for Cell Surface Protein library)


- i. Vortex to resuspend the SPRIselect reagent. Add **70 µl** SPRIselect reagent (**2.0X**) to **80 µl** of the transferred supernatant and pipette mix 15x (pipette set to 150 µl).
- ii. Incubate for **5 min** at **room temperature**.
- iii. Place on the magnet•**High** until the solution clears.
- iv. Remove the supernatant.
- v. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- vi. Remove the ethanol.
- vii. **Repeat** steps v and vi for a total of 2 washes.
- viii. Centrifuge briefly and place on the magnet•**Low**.
- ix. Remove any remaining ethanol. Air dry for **2 min**. DO NOT exceed **2 min** as this will decrease elution efficiency.
- x. Remove from the magnet. Add **45.5 µl** Buffer EB. Pipette mix 15x.
- xi. Incubate **2 min** at **room temperature**.
- xii. Place the tube strip on the magnet•**High** until the solution clears.
- xiii. Transfer **45 µl** sample to a new tube strip.
- xiv.  Store at **4°C** for up to **72 h** or at **–20°C** for up to a **week**, or proceed directly to **step 7 for Cell Surface Protein Library Construction**.

3.3 cDNA QC & Quantification



For 5' Gene Expression Library Construction proceed directly to step 6 after step 3.3.

- a. Run 1 μL undiluted sample from the Pellet Cleanup step 3.2A-x (Dilution Factor 1) on an Agilent Bioanalyzer High Sensitivity chip.

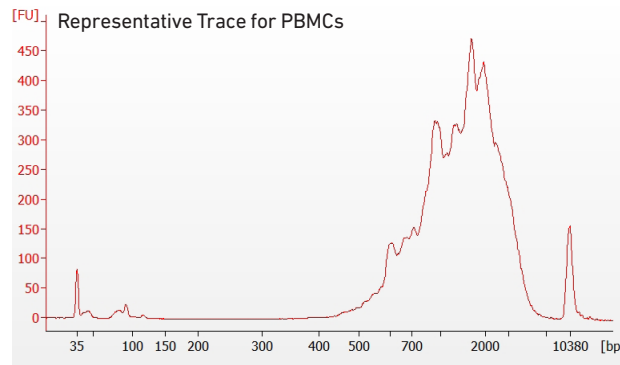


- b. If proceeding to 5' GEX Library Construction (step 6), determine cDNA yield for each sample. Example calculation below.


EXAMPLE CALCULATION

i. Select Region

Under the "Electropherogram" view choose the "Region Table". Manually select the region of ~200 – ~9000 bp

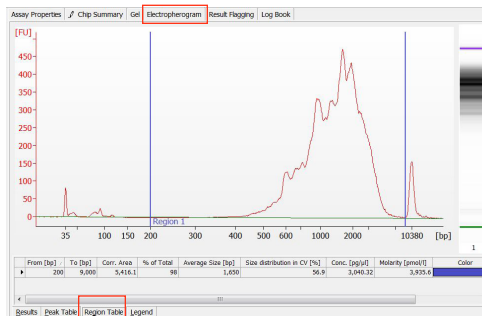

ii. Note Concentration [pg/μL]

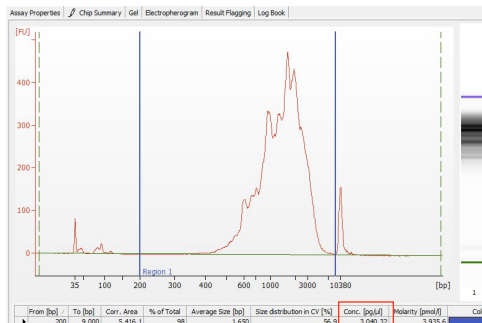

iii. Calculate

Concentration: 3040.32 pg/μL

Dilution Factor: 1

cDNA Conc. =

$$\text{Conc. (pg/μL)} \times \text{Dilution Factor} = \frac{3040.32 \times 1}{1000 \text{ (pg/ng)}} = \frac{3040.32}{1000} = 3 \text{ ng/μL}$$

Example Calculation for Carrying Forward 50 ng Sample for 5' GEX Library Construction

$$\text{Volume for 50 ng} = \frac{50 \text{ ng}}{3 \text{ (ng/μL)}} = 16.7 \mu\text{L}$$

5' GEX Library Construction Sample
= 16.7 μL + 3.3 μL nuclease-free water
= 20 μL total

If <50 ng available, carry forward 20 μL sample (2-50 ng) into 5' GEX Library Construction.



DO NOT exceed a mass of 50 ng in the 20 μL carry forward volume.

Alternate Quantification Methods:











- Agilent TapeStation. See Appendix for representative traces
- Qubit Fluorometer and Qubit dsDNA HS Assay Kit.

Step 4

Target Enrichment from cDNA

- 4.1 Target Enrichment 1
- 4.2 Post Target Enrichment 1 Cleanup – SPRIselect
- 4.3 Target Enrichment 2
- 4.4 Post Target Enrichment 2 Double Sided Size Selection – SPRIselect
- 4.5 Post Target Enrichment QC & Quantification





4.0 Target Enrichment from cDNA

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	For Human Samples (Choose B or T-cell primers based on desired enrichment products)			
	 Human T Cell Mix 1	2000008	Vortex, centrifuge briefly.	-20°C
	 Human T Cell Mix 2	2000009	Vortex, centrifuge briefly.	-20°C
	 Human B Cell Mix 1	2000035	Vortex, centrifuge briefly.	-20°C
	 Human B Cell Mix 2	2000036	Vortex, centrifuge briefly.	-20°C
	For Mouse Samples (Choose B or T-cell primers based on desired enrichment products)			
	 Mouse T Cell Mix 1	2000075	Vortex, centrifuge briefly.	-20°C
	 Mouse T Cell Mix 2	2000079	Vortex, centrifuge briefly.	-20°C
	 Mouse B Cell Mix 1	2000080	Vortex, centrifuge briefly.	-20°C
	 Mouse B Cell Mix 2	2000081	Vortex, centrifuge briefly.	-20°C
	For all Samples			
	 cDNA Additive	220067	Vortex, centrifuge briefly.	-20°C
	Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
	Agilent Bioanalyzer High Sensitivity Kit If used for QC and quantification	-	Manufacturer's recommendations.	-
	Agilent TapeStation ScreenTape and Reagents If used for QC and quantification	-	Manufacturer's recommendations.	-
	Qubit dsDNA HS Assay Kit If used for quantification	-	Manufacturer's recommendations.	-
Place on Ice	 Amplification Master Mix	220125	Vortex, centrifuge briefly.	-20°C
Obtain	Qiagen Buffer EB	-	-	Ambient
	10x Magnetic Separator	230003	See Tips & Best Practices.	Ambient
	Prepare 80% Ethanol Prepare 15 ml for 8 reactions	-	See Tips & Best Practices.	Ambient

4.1

Target Enrichment 1

- a. Add 33 μ l nuclease-free water into a tube strip on ice and then transfer 2 μ l sample (post cDNA Amplification & QC, step 3.3) to the same tube for a total of 35 μ l.
- b. Prepare Target Enrichment 1 Reaction Mix on ice. Vortex and centrifuge briefly.

Target Enrichment 1 Reaction Mix <i>Add reagents in the order listed</i>	PN	1X (μ l)	4X + 10% (μ l)	8X + 10% (μ l)
Nuclease-free Water	-	5	22	44
 Amplification Master Mix	220125	50	220	440
 cDNA Additive	220067	5	22	44
 T Cell Mix 1	Human 2000008/ Mouse 2000075	5	22	44
or	or			
 B Cell Mix 1	Human 2000035/ Mouse 2000080			
Total	-	65	286	572

- c. Add 65 μ l Target Enrichment 1 Reaction Mix to each tube containing 35 μ l sample.
- d. Pipette mix 5x (pipette set to 90 μ l). Centrifuge briefly.
- e. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μ l	~20-30 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	67°C	00:00:30
4	72°C	00:01:00
5	T Cell: Go to Step 2, 9x (total 10 cycles) B Cell: Go to Step 2, 5x (total 6 cycles)	
6	72°C	00:01:00
7	4°C	Hold



Different cycle numbers for T & B cells



- f. Store at 4°C for up to 72 h or proceed to the next step.

4.2





Post Target Enrichment 1 Cleanup – SPRIselect

- a. Vortex to resuspend the SPRIselect reagent. Add **80 µl** SPRIselect reagent (**0.8X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place tube strip on the magnet•**High** until the solution clears.
- d. Remove the supernatant.
- e. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- f. Remove the ethanol.
- g. **Repeat** steps e and f for a total of 2 washes.
- h. Centrifuge briefly. Place on the magnet•**Low**.
- i. Remove remaining ethanol. Air dry for **2 min**.
- j. Remove from the magnet. Add **35.5 µl** Buffer EB. Pipette mix 15x.
- k. Incubate **2 min** at **room temperature**.
- l. Place on the magnet•**Low** until the solution clears.
- m. Transfer **35 µl** sample to a new tube strip.
- n. Store at **4°C** in for up to **72 h** or at **-20°C** for up to a **week**, or proceed to the next step.



4.3 Target Enrichment 2

a. Prepare Target Enrichment 2 Reaction Mix on ice. Vortex and centrifuge briefly.

Target Enrichment 2 Reaction Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
Nuclease-free Water	-	5	22	44
 Amplification Master Mix	220125	50	220	440
 cDNA Additive	220067	5	22	44
 T Cell Mix 2	Human 2000009/ Mouse 2000079	5	22	44
or	or			
 B Cell Mix 2	Human 2000036/ Mouse 2000081			
Total	-	65	286	572

c. Add 65 μl Target Enrichment 2 Reaction Mix to each tube containing 35 μl sample.

d. Pipette mix 5x (pipette set to 90 μl). Centrifuge briefly.

e. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~25-30 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	67°C	00:00:30
4	72°C	00:01:00
5	T Cell: Go to Step 2, 9x (total 10 cycles) B Cell: Go to Step 2, 7x (total 8 cycles)	
6	72°C	00:01:00
7	4°C	Hold



Different cycle numbers for T & B cells



f. Store at 4°C for up to 72 h or proceed to the next step.

4.4
Post Target Enrichment 2
Double Sided Size
Selection – SPRIselect

- a. Vortex to resuspend SPRIselect reagent. Add **50 µl** SPRIselect reagent (**0.5X**) to each sample. Pipette mix 15x (pipette set to 145 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears. DO NOT discard supernatant.
- d. Transfer **145 µl** supernatant to a new tube strip.
- e. Vortex to resuspend SPRIselect reagent. Add **30 µl** SPRIselect reagent (**0.8X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- f. Incubate **5 min** at **room temperature**.
- g. Place on the magnet•**High** until the solution clears.
- h. Remove **170 µl** supernatant. DO NOT discard any beads.
- i. Add **200 µl** 80% ethanol. Wait **30 sec**.
- j. Remove the ethanol.
- k. **Repeat** steps i and j for a total of 2 washes.
- l. Centrifuge briefly. Place on the magnet•**Low**.
- m. Remove remaining ethanol wash. DO NOT over-dry beads to ensure maximum elution efficiency.
- n. Remove from the magnet. Add **45.5 µl** Buffer EB. Pipette mix 15x.
- o. Incubate **2 min** at **room temperature**.
- p. Place on the magnet•**Low** until the solution clears.
- q. Transfer **45 µl** sample to a new tube strip.
- r. Store at **4°C** for up to **72 h** or at **-20°C** for up to **1 week**, or proceed to the next step.




4.5 Post Target Enrichment QC & Quantification


a. Run 1 µl sample at 1:5 dilution (Dilution Factor 5) on an Agilent Bioanalyzer High Sensitivity chip.

Samples of RNA-rich cells may require additional dilution in nuclease-free water. The number of distinct peaks may vary. Higher molecular weight product (2,000– 9,000 bp) may be present. This does not affect sequencing.

Representative Trace - PBMCs enriched for TCR

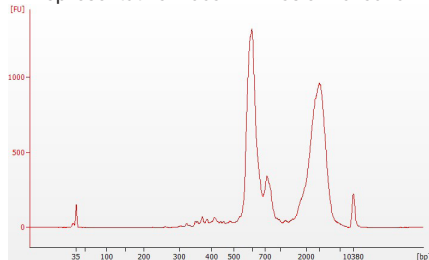

Representative Trace - PBMCs enriched for Ig

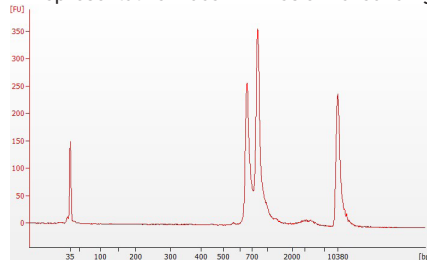


b. Determine yield for each sample. Example calculation below.


EXAMPLE CALCULATION

i. Select Region

Under the “Electropherogram” view choose the “Region Table”. Manually select the region of ~200 – ~9000 bp.

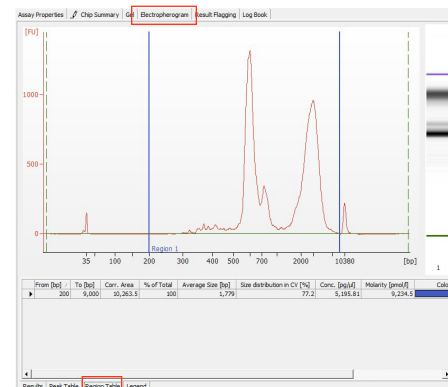

ii. Note Concentration [pg/µl]

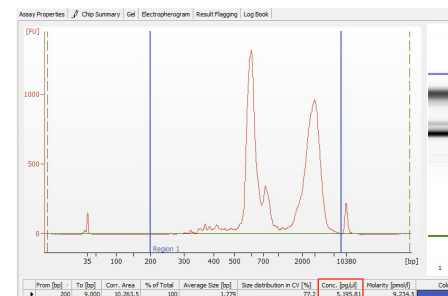

iii. Calculate

Concentration: 5195.81 pg/µl

Dilution Factor: 5

Enriched Product Conc.

$$\text{Conc. (pg/µl)} \times \text{Dilution Factor} = \frac{5195.81 \times 5}{1000 \text{ (pg/ng)}} = \frac{25979.05}{1000} = 26 \text{ ng/µl}$$

Example Calculation for Carrying Forward 50 ng Sample for Enriched Library Construction

$$\text{Volume for 50 ng} = \frac{50 \text{ ng}}{26 \text{ (ng/µl)}} = 1.9 \text{ µl}$$

Enriched Library Construction Sample
= 1.9 µl + 18.1 µl nuclease-free water
= 20 µl total

If <50 ng available, carry forward 20 µl sample (2–50 ng) into Enriched Library Construction.



DO NOT exceed a mass of 50 ng in the 20 µl carry forward volume.

Alternate Quantification Methods:

- Agilent TapeStation. [See Appendix for representative traces](#)
- Qubit Fluorometer and Qubit dsDNA HS Assay Kit.










Step 5

Enriched Library Construction

- 5.1 Fragmentation, End Repair & A-tailing
- 5.2 Adaptor Ligation
- 5.3 Post Ligation Cleanup – SPRIselect
- 5.4 Sample Index PCR
- 5.5 Post Sample Index PCR Cleanup – SPRIselect
- 5.6 Post Library Construction QC



5.0 Enriched Library Construction

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	 Fragmentation Buffer	220108	Thaw, vortex, verify no precipitate, centrifuge briefly.	-20°C
	 Adaptor Mix	220026	Vortex, centrifuge briefly.	-20°C
	 Ligation Buffer	220109	Thaw, vortex, verify no precipitate, centrifuge briefly.	-20°C
	 SI-PCR Primer  Verify name & PN (Different from step 7)	220111	Vortex, centrifuge briefly.	-20°C
	 Chromium i7 Sample Index Plate Verify name & PN (Different from step 7)	220103	-	-20°C
	Beckman Coulter SPRiselect Reagent	-	Manufacturer's recommendations.	-
	Agilent Bioanalyzer High Sensitivity Kit If used for QC	-	Manufacturer's recommendations.	-
	Agilent TapeStation ScreenTape and Reagents If used for QC	-	Manufacturer's recommendations.	-
Place on Ice	 Fragmentation Enzyme Blend	220107/ 220130	Centrifuge briefly.	-20°C
	 DNA Ligase	220110/ 220131	Centrifuge briefly.	-20°C
	 Amplification Master Mix	220125	Vortex, centrifuge briefly.	-20°C
Obtain	Qiagen Buffer EB	-	-	Ambient
	10x Magnetic Separator	230003	See Tips & Best Practices.	Ambient
	Prepare 80% Ethanol Prepare 15 ml for 8 reactions	-	Prepare fresh.	Ambient

5.1 Fragmentation, End Repair & A-tailing

- a. Determine the volume for **50 ng** mass of sample (see example calculation at step 4.5). Dispense the sample volume in a tube strip **on ice**. If the volume required for **50 ng** is less than **20 µl**, adjust the total volume of each sample to **20 µl** with nuclease-free water. If the volume for **50 ng** exceeds **20 µl**, carry only **20 µl** sample into library construction.
- b. Prepare a thermal cycler with the following incubation protocol.



Lid Temperature	Reaction Volume	Run Time
65°C	50 µl	~35 min
Step	Temperature	Time
Pre-cool block <i>Pre-cool block prior to preparing the Fragmentation Mix</i>	4°C	Hold
Fragmentation	32°C	00:02:00
End Repair & A-tailing	65°C	00:30:00
Hold	4°C	Hold




- c. Vortex Fragmentation Buffer. Verify there is no precipitate.
- d. Prepare Fragmentation Mix on ice. Pipette mix and centrifuge briefly.

Fragmentation Mix <i>Add reagents in the order listed</i>	PN	1X (µl)	4X + 10% (µl)	8X + 10% (µl)
Nuclease-free Water	-	15	66	132
<input type="radio"/> Fragmentation Buffer	220108	5	22	44
<input checked="" type="radio"/> Fragmentation Enzyme Blend	220107/ 220130	10	44	88
Total	-	30	132	264

- e. Add **30 µl** Fragmentation Mix into each tube containing **20 µl** sample.
- f. Pipette mix 15x (pipette set to 30 µl) on ice. Centrifuge briefly.
- g. Transfer into the pre-cooled thermal cycler (**4°C**) and press “SKIP” to initiate the protocol.

5.2 Adaptor Ligation

a. Prepare Adaptor Ligation Mix. Pipette mix and centrifuge briefly.

Adaptor Ligation Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
Nuclease-free Water	-	17.5	77	154
 Ligation Buffer	220109	20	88	176
 DNA Ligase	220110/ 220131	10	44	88
 Adaptor Mix	220026	2.5	11	22
Total	-	50	220	440

b. Remove the sample from the thermal cycler.

c. Add 50 μl Adaptor Ligation Mix to 50 μl sample. Pipette mix 15x (pipette set to 90 μl). Centrifuge briefly.

d. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
30°C	100 μl	15 min
Step	Temperature	Time
1	20°C	00:15:00
2	4°C	Hold

5.3 Post Ligation Cleanup – SPRIselect



- a. Vortex to resuspend SPRIselect Reagent. Add **80 µl** SPRIselect Reagent (**0.8X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears.
- d. Remove the supernatant.
- e. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- f. Remove the ethanol.
- g. **Repeat** steps e and f for a total of 2 washes.
- h. Centrifuge briefly. Place on the magnet•**Low**.
- i. Remove any remaining ethanol. Air dry for **2 min**.
- j. Remove from the magnet. Add **30.5 µl** Buffer EB. Pipette mix 15x. If beads still appear clumpy, continue pipette mixing until fully resuspended.
- k. Incubate **2 min** at **room temperature**.
- l. Place on the magnet•**Low** until the solution clears.
- m. Transfer **30 µl** sample to a new tube strip.

5.4 Sample Index PCR



- a. Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run.
Record the 10x Sample Index name (PN-220103 Chromium i7 Sample Index Plate well ID) used.

- b. Prepare Sample Index PCR Mix.

Sample Index PCR Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
Nuclease-free Water	-	8	35	70
 Amplification Master Mix	220125	50	220	440
 SI-PCR Primer <i>Verify name & PN</i>	220111	2	9	18
Total	-	60	264	528



- c. Add 60 μl Sample Index PCR Mix to 30 μl sample.
- d. Add 10 μl of an individual Chromium i7 Sample Index to each well and record the well ID. Pipette mix 5x (pipette set to 90 μl). Centrifuge briefly.
- e. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~30 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	54°C	00:00:30
4	72°C	00:00:20
5	Go to step 2, 8x (total 9 cycles)	
6	72°C	00:01:00
7	4°C	Hold



- f. Store at 4°C for up to 72 h or proceed to the next step.

5.5

Post Sample Index PCR Cleanup – SPRIselect


- a. Vortex to resuspend the SPRIselect reagent. Add **80 µl** SPRIselect Reagent (**0.8X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place the magnet•**High** until the solution clears.
- d. Remove the supernatant.
- e. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- f. Remove the ethanol.
- g. **Repeat** steps e and f for a total of 2 washes.
- h. Centrifuge briefly. Place on the magnet•**Low**.
- i. Remove remaining ethanol. Air dry for **2 min**.
- j. Remove from the magnet. Add **35.5 µl** Buffer EB. Pipette mix 15x.
- k. Incubate **2 min** at **room temperature**.
- l. Place on the magnet•**Low** until the solution clears.
- m. Transfer **35 µl** to a new tube strip.
- n. Store at **4°C** for up to **72 h** or at **-20°C** for **long-term** storage.




5.6 Post Library Construction QC

a. Run 1 μ l sample at 1:10 dilution on an Agilent Bioanalyzer High Sensitivity chip.

Representative Trace - PBMCs enriched for TCR

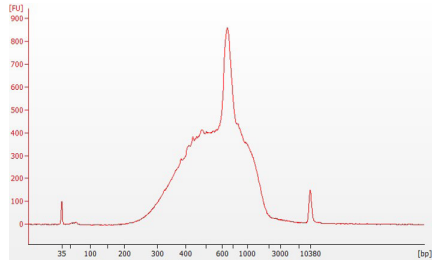

Representative Trace - PBMCs enriched for Ig

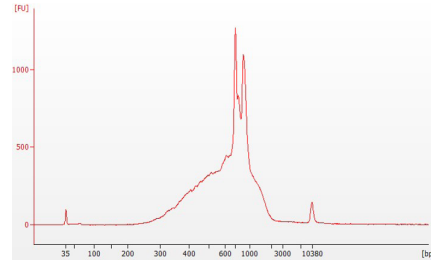

b. Determine the average fragment size from the trace. This will be used as the insert size for library quantification.

Alternate QC Method:

- Agilent TapeStation. [See Appendix for representative traces](#)










[See Appendix for Post Library Construction Quantification](#)

Step 6

5' Gene Expression (GEX) Library Construction

- 6.1** GEX Fragmentation, End Repair & A-tailing
- 6.2** GEX Post Fragmentation, End Repair & A-tailing
Double Sided Size Selection – SPRIselect
- 6.3** GEX Adaptor Ligation
- 6.4** GEX Post Ligation Cleanup – SPRIselect
- 6.5** GEX Sample Index PCR
- 6.6** GEX Post Sample Index Double Sided
Size Selection – SPRIselect
- 6.7** GEX Post Library Construction QC

6.0 5' Gene Expression (GEX) Library Construction

GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	 Fragmentation Buffer	220108	Thaw, vortex, verify no precipitate, centrifuge briefly.	-20°C
	 Adaptor Mix	220026	Vortex, centrifuge briefly.	-20°C
	 Ligation Buffer	220109	Thaw, vortex, verify no precipitate, centrifuge briefly.	-20°C
	 SI-PCR Primer	220111	Vortex, centrifuge briefly.	-20°C
	 Chromium i7 Sample Index Plate Verify name & PN (Different from step 7)	220103	-	-20°C
	 Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
	Agilent Bioanalyzer DNA 1000 kit If used for QC	-	Manufacturer's recommendations.	-
	Agilent TapeStation ScreenTape and Reagents If used for QC	-	Manufacturer's recommendations.	-
Place on Ice	 Fragmentation Enzyme Blend	220107/ 220130	Centrifuge briefly.	-20°C
	 DNA Ligase	220110/ 220131	Centrifuge briefly.	-20°C
	 Amplification Master Mix	220125	Vortex, centrifuge briefly.	-20°C
Obtain	Qiagen Buffer EB	-	-	Ambient
	10x Magnetic Separator	230003	See Tips & Best Practices.	Ambient
	Prepare 80% Ethanol Prepare 15 ml for 8 reactions	-	Prepare fresh.	Ambient

6.1 GEX Fragmentation, End Repair & A-tailing

- a. Determine the volume for **50 ng** mass of sample (see example calculation at step 3.3). Dispense the sample volume in a tube strip **on ice**. If the volume required for **50 ng** is less than **20 µl**, adjust the total volume of each sample to **20 µl** with nuclease-free water. If the volume for **50 ng** exceeds **20 µl**, carry **ONLY 20 µl** sample into library construction.
- b. Prepare a thermal cycler with the following incubation protocol.

Lid Temperature	Reaction Volume	Run Time
65°C	50 µl	~35 min

Step	Temperature	Time
Pre-cool block <i>Pre-cool block prior to preparing the Fragmentation Mix</i>	4°C	Hold
Fragmentation	32°C	00:05:00
End Repair & A-tailing	65°C	00:30:00
Hold	4°C	Hold

- c. Vortex Fragmentation Buffer. Verify there is no precipitate.
- d. Prepare Fragmentation Mix on ice. Pipette mix and centrifuge briefly.

Fragmentation Mix <i>Add reagents in the order listed</i>	PN	1X (µl)	4X + 10% (µl)	8X + 10% (µl)
Nuclease-free Water	-	15	66	132
<input type="radio"/> Fragmentation Buffer	220108	5	22	44
<input checked="" type="radio"/> Fragmentation Enzyme Blend	220107/ 220130	10	44	88
Total	-	30	132	264




- e. Add **30 µl** Fragmentation Mix into each tube containing **20 µl** sample.
- f. Pipette mix 15x (pipette set to 30 µl) on ice. Centrifuge briefly.
- g. Transfer into the pre-cooled thermal cycler (**4°C**) and press “SKIP” to initiate the protocol.

6.2
GEX Post Fragmentation,
End Repair & A-tailing
Double Sided Size
Selection – SPRIselect

- a. Vortex to resuspend SPRIselect Reagent. Add 30 μ l SPRIselect Reagent (**0.6X**) to each sample. Pipette mix 15x (pipette set to 75 μ l).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet •**High** until the solution clears. **DO NOT** discard supernatant.
- d. Transfer **75 μ l** supernatant to a new tube strip.
- e. Add **10 μ l** SPRIselect reagent (**0.8X**) to each sample. Pipette mix 15x (pipette set to 75 μ l).
- f. Incubate **5 min** at **room temperature**.
- g. Place on the magnet •**High** until the solution clears.
- h. Remove **80 μ l** supernatant. **DO NOT** discard any beads.
- i. With the tube strip still on the magnet, add **125 μ l** 80% ethanol to the pellet. Wait **30 sec**.
- j. Remove the ethanol.
- k. **Repeat** steps i and j for a total of 2 washes.
- l. Centrifuge briefly. Place on the magnet •**Low**.
- m. Remove the ethanol. **DO NOT** over-dry beads to ensure maximum elution efficiency.
- n. Remove from the magnet. Add **50.5 μ l** Buffer EB. Pipette mix 15x.
- o. Incubate **2 min** at **room temperature**.
- p. Place on the magnet •**High** until the solution clears.
- q. Transfer **50 μ l** sample to a new tube strip.

6.3 GEX Adaptor Ligation

a. Prepare Adaptor Ligation Mix. Pipette mix and centrifuge briefly.

Adaptor Ligation Mix <i>Add reagents in the order listed</i>	PN	1X (µl)	4X + 10% (µl)	8X + 10% (µl)
Nuclease-free Water	-	17.5	77	154
 Ligation Buffer	220109	20	88	176
 DNA Ligase	220110/ 220131	10	44	88
 Adaptor Mix	220026	2.5	11	22
Total	-	50	220	440

b. Add 50 µl Adaptor Ligation Mix to 50 µl sample. Pipette mix 15x (pipette set to 90 µl). Centrifuge briefly.

c. Incubate in a thermal cycler with the following protocol.




Lid Temperature	Reaction Volume	Run Time
30°C	100 µl	15 min
Step	Temperature	Time
1	20°C	00:15:00
2	4°C	Hold

6.4
GEX Post
Ligation Cleanup –
SPRIselect

- a. Vortex to resuspend SPRIselect Reagent. Add **80 µl** SPRIselect Reagent (**0.8X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears.
- d. Remove the supernatant.
- e. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- f. Remove the ethanol.
- g. **Repeat** steps e and f for a total of 2 washes.
- h. Centrifuge briefly. Place on the magnet•**Low**.
- i. Remove any remaining ethanol. Air dry for **2 min**.
- j. Remove from the magnet. Add **30.5 µl** Buffer EB. Pipette mix 15x.
- k. Incubate **2 min** at **room temperature**.
- l. Place on the magnet•**Low** until the solution clears.
- m. Transfer **30 µl** sample to a new tube strip.

6.5 GEX Sample Index PCR

- Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run.
- Record the 10x Sample Index name (PN-220103 Chromium i7 Sample Index Plate well ID) used.
- Prepare Sample Index PCR Mix. Pipette mix and centrifuge briefly.

Sample Index PCR Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
Nuclease-free Water	-	8	35	70
 Amplification Master Mix	220125	50	220	440
  SI-PCR Primer <i>Verify name & PN</i>	220111	2	9	18
Total	-	60	264	528

- Add 60 μl Sample Index PCR Mix to 30 μl sample.
- Add 10 μl of an individual Chromium i7 Sample Index to each well and record the well ID. Pipette mix 5x (pipette set to 90 μl). Centrifuge briefly.
- Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~40 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	54°C	00:00:30
4	72°C	00:00:20
5	Go to step 2, see table below for # cycles	
6	72°C	00:01:00
7	4°C	Hold

The table recommends starting point for optimization. If less than 50 ng was carried into 5' Gene Expression Library Construction, refer to the product yield calculation example in step 3.3 to determine the mass input into Library Construction.

Input into Library Construction	Total Sample Index Cycles
1-25 ng	16
26-50 ng	14



- Store at 4°C for up to 72 h or proceed to the next step.


6.6
GEX Post Sample Index
PCR Double Sided Size
Selection – SPRIselect

- a. Vortex to resuspend SPRIselect reagent. Add **60 µl** SPRIselect reagent (**0.6X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place on the magnet•**High** until the solution clears. **DO NOT** discard supernatant.
- d. Transfer **150 µl** supernatant to a new tube strip.
- e. Vortex to resuspend SPRIselect reagent. Add **20 µl** SPRIselect reagent (**0.8X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- f. Incubate **5 min** at **room temperature**.
- g. Place on the magnet•**High** until the solution clears.
- h. Remove **165 µl** supernatant. **DO NOT** discard any beads.
- i. With the tube strip still on the magnet, add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- j. Remove the ethanol.
- k. **Repeat** steps i and j for a total of 2 washes.
- l. Centrifuge briefly. Place on the magnet•**Low**.
- m. Remove the remaining ethanol. **DO NOT** over-dry beads to ensure maximum elution efficiency.
- n. Remove the tube strip from the magnet. Add **35.5 µl** Buffer EB. Pipette mix 15x.
- o. Incubate **2 min** at **room temperature**.
- p. Place on the magnet•**Low** until the solution clears.
- q. Transfer **35 µl** sample to a new tube strip.
- r. Store at **4°C** for up to **72 h** or at **-20°C** for **long-term** storage.



6.7 GEX Post Library Construction QC

a. Run 1 μL sample at 1:10 dilution on an Agilent Bioanalyzer High Sensitivity chip.

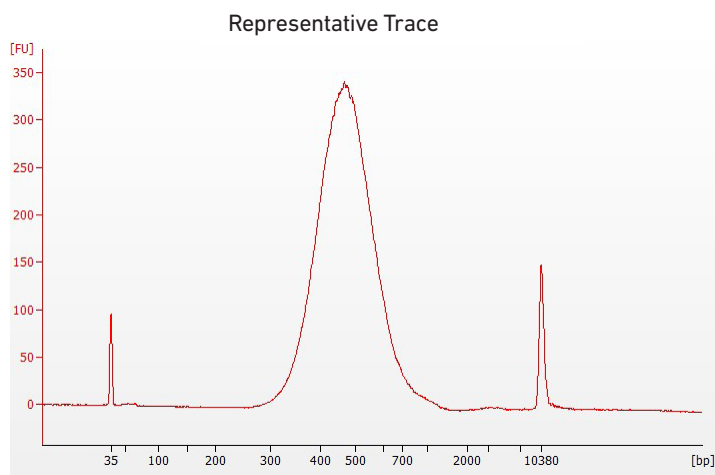

b. Determine the average fragment size from the trace. This will be used as the insert size for library quantification.

Alternate QC Method:

- Agilent TapeStation. [See Appendix for representative traces](#)

[See Appendix for Post Library Construction Quantification](#)





Step 7

Cell Surface Protein Library Construction

- 7.1 Sample Index PCR
- 7.2 Post Sample Index PCR Size Selection – SPRIselect
- 7.3 Post Library Construction QC



7.0 Cell Surface Protein Library Construction



GET STARTED!				
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	 SI Primer  Verify name & PN (Different from steps 5 & 6)	2000095	-	-20°C
	Chromium i7 Sample Index Plate N, Set A  Verify name & PN (Different from steps 5 & 6)	3000262	-	-20°C
	Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
	Agilent TapeStation Screen Tape and Reagents If used for QC	-	Manufacturer's recommendations.	-
	Agilent Bioanalyzer High Sensitivity kit If used for QC	-	Manufacturer's recommendations.	-
Place on ice	 Amplification Master Mix	220125	Vortex, centrifuge briefly.	-20°C
	KAPA Library Quantification Kit for Illumina Platforms	-	Manufacturer's recommendations.	-
Obtain	Qiagen Buffer EB	-	-	Ambient
	10x Magnetic Separator	230003	See Tips & Best Practices	Ambient
	Prepare 80% Ethanol Prepare 20 ml for 8 reactions	-	Prepare fresh.	Ambient

7.1 Sample Index PCR



a. Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run. Record the 10x Sample Index name (PN-3000262 Chromium i7 Sample Index Plate N, Set A well ID; verify name and part number) used.

b. Prepare Sample Index PCR Mix.

Sample Index PCR Mix <i>Add reagents in the order listed</i>	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
Nuclease-free Water		25	110	220
 Amplification Master Mix	220125	50	220	440
 SI Primer <i>Verify name & PN</i>	2000095	10	44	88
Total	-	85	374	748



c. Transfer **ONLY 5 μl** sample from the Transferred Supernatant Cleanup (step 3.2B-xiv) to a new tube strip.

Note that only **5 μl** of the DNA sample is adequate for generating Cell Surface Protein library. The remaining DNA sample can be stored at **4°C** for up to **72 h** or at **-20°C** for up to a **week** for generating additional Cell Surface Protein libraries.

d. Add **85 μl** Sample Index PCR Mix to the **5 μl** Transferred Supernatant Cleanup sample.

e. Add **10 μl** of an individual Chromium i7 Sample indices N, Set A to each well and record the well ID. Pipette mix 5x (pipette set to 90 μl). Centrifuge briefly.

f. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~30 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	54°C	00:00:30
4	72°C	00:00:20
5	Go to step 2, repeat 8X (total 9 cycles)*	
6	72°C	00:01:00
7	4°C	Hold

*Optimization of cycle number may be needed based on target protein expression levels and number of antibodies used for labeling.


7.2
Post Sample Index
PCR Size Selection –
SPRIselect

- a. Vortex to resuspend the SPRIselect reagent. Add **120 µl** SPRIselect Reagent (**1.2X**) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate **5 min** at **room temperature**.
- c. Place the magnet•**High** until the solution clears. Remove the supernatant.
- d. Add **300 µl** 80% ethanol to the pellet. Wait **30 sec**.
- e. Remove the ethanol.
- f. Add **200 µl** 80% ethanol to the pellet. Wait **30 sec**.
- g. Remove the ethanol.
- h. Centrifuge briefly. Place on the magnet•**Low**. Remove remaining ethanol.
- i. Remove from the magnet. Add **35.5 µl** Buffer EB. Pipette mix 15x.
- j. Incubate **2 min** at **room temperature**.
- k. Place on the magnet•**Low** until the solution clears.
- l. Transfer **35 µl** to a new tube strip.
- m. Store at **4°C** for up to **72 h** or at **-20°C** for **long-term** storage.



7.3 Post Library Construction QC

Run 1 μ l sample at 1:10 dilution on an Agilent Bioanalyzer High Sensitivity chip.

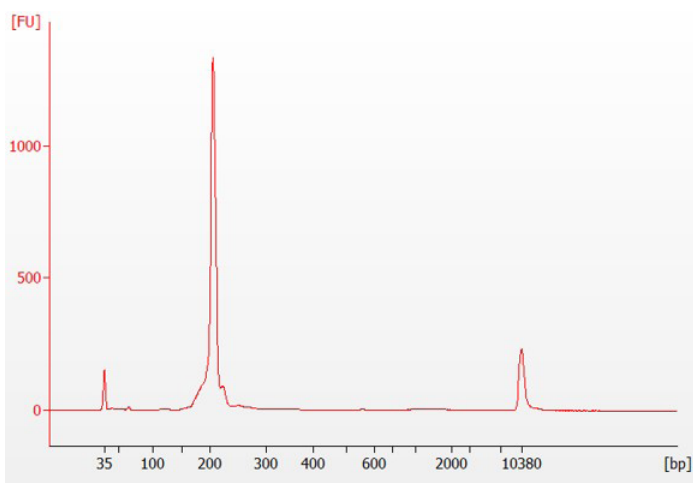

Determine the average fragment size from the Bioanalyzer trace. This will be used as the insert size for library quantification.

Alternate QC Method:

- Agilent TapeStation. [See Appendix for representative traces](#)

[See Appendix for Post Library Construction Quantification](#)

Sequencing



Sequencing Libraries

Chromium Single Cell V(D)J Enriched libraries, 5' Gene Expression libraries, and Cell Surface Protein libraries comprise standard Illumina paired-end constructs which begin with P5 and end with P7. These libraries include 16 bp 10x Barcodes encoded at the start of TruSeq Read 1. Sample index sequences are incorporated as the i7 index read for V(D)J Enriched and 5' Gene Expression libraries; as i7 index read N for Cell Surface Protein library. TruSeq Read 1, TruSeq Read 2, and Nextera Read 2 (Read 2N) are all standard Illumina sequencing primer sites. TruSeq Read 1 and TruSeq Read 2 are used in paired-end sequencing of V(D)J Enriched and 5' Gene Expression libraries. TruSeq Read 1 and Nextera Read 2 (Read 2N) are used for paired-end sequencing of Cell Surface Protein library. Sequencing these libraries produce a standard Illumina BCL data output folder.

Chromium Single Cell V(D)J Enriched Library



Chromium Single Cell 5' Gene Expression Library



Chromium Single Cell 5' Cell Surface Protein Library



Illumina Sequencer Compatibility

The compatibility of the listed sequencers has been verified by 10x Genomics. Some variation in assay performance is expected based on sequencer choice. For more information about performance variation, visit the 10x Genomics Support website.

- MiSeq
- NextSeq 500/550*
- HiSeq 2500 (Rapid Run)
- HiSeq 3000/4000
- NovaSeq

*Sequencing Chromium Single Cell libraries on the NextSeq 500/550 platform may yield reduced sequence quality and sensitivity relative to the MiSeq, HiSeq, and NovaSeq platforms. Refer to the 10x Genomics Support website for more information.

Sample Indices

Each sample index in the Chromium i7 Sample Index Kit (PN-120262) and Chromium i7 Sample Index Kit Plate N, Set A (PN-1000084) is a mix of 4 different sequences to balance across all 4 nucleotides. If multiple samples are pooled in a sequence lane, the sample index name (i.e. the Chromium i7 Sample Index plate well ID) is needed in the sample sheet used for generating FASTQs with "cellranger mkfastq". If multiple libraries are pooled in a sequence lane, a separate sample index is needed with each library (see [Tips & Best Practices](#)).

Library Sequencing Depth & Run Parameters

Sequencing Depth	Minimum 5,000 read pairs per cell for V(D)J Enriched library	
	Minimum 20,000 read pairs per cell for 5' Gene Expression library	
	Minimum 5,000 read pairs per cell for Cell Surface Protein library	
Sequencing Type	Paired-end, single indexing	
Sequencing Read	Recommended Cycles	
	Read 1	Read 2
V(D)J Enriched library	150	150
5' Gene Expression library	26	91
Cell Surface Protein library	26	25
5' Gene Expression + Cell Surface Protein libraries	26	91
V(D)J Enriched + 5' Gene Expression	150	150
V(D)J Enriched + 5' Gene Expression + Cell Surface Protein libraries	150	150

Library Loading

Once quantified and normalized, V(D)J Enriched, 5' Gene Expression, and Cell Surface Protein libraries should be denatured and diluted as recommended for Illumina sequencing platforms. Refer to Illumina documentation for denaturing and diluting libraries. Refer to the 10x Genomics Support website, for more information.

Instrument	Loading Concentration (pM)	PhiX (%)
MiSeq	10	1
NextSeq 500	1.5	1
HiSeq 2500 (RR)	10	1
HiSeq 4000	180	1
NovaSeq	200	1

Library Pooling

V(D)J Enriched, 5' Gene Expression, and Cell Surface Protein libraries may be pooled for sequencing, taking into account the differences in depth requirements between the pooled libraries.

Library Pooling Examples:





Libraries	Sequencing Depth (read pairs per cell)	Library Pooling Ratio
Example 1		
V(D)J Enriched library	5,000	1
5' Gene Expression library	20,000	4
Cell Surface Protein library	5,000	1
Example 2		
V(D)J Enriched library	5,000	1
5' Gene Expression library	50,000	10
Cell Surface Protein library	5,000	1


Troubleshooting



9

GEMs

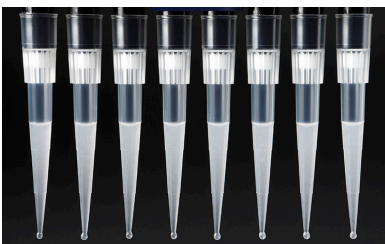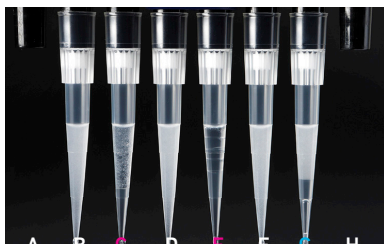STEP	NORMAL	REAGENT CLOGS & WETTING FAILURES
<p>1.4 d</p> <p>After Chip G is removed from the Controller and the wells are exposed</p>	 <p>All 8 recovery wells are similar in volume and opacity.</p>	 <p>Recovery well G indicates a reagent clog. Recovery well C and E indicate a wetting failure. Recovery wells B, D, and F are normal. Wells A and H contain 50% Glycerol Solution.</p>
<p>1.4 e</p> <p>Transfer GEMs from Chip G Recovery Wells</p>	 <p>All liquid levels are similar in volume and opacity without air trapped in the pipette tips.</p>	 <p>Pipette tips C and E indicate a wetting failure. Pipette tip C contains partially emulsified GEMs. Emulsion is absent in pipette tip E. Pipette tip G indicates a reagent clog.</p>

STEP	NORMAL	REAGENT CLOGS & WETTING FAILURES
<p>2.1 a</p> <p>After transfer of the GEMs + Recovery Agent</p>	 <p>All liquid levels are similar in the aqueous sample volume (clear) and Recovery Agent/Partitioning Oil (pink).</p>	 <p>Tube G indicates a reagent clog has occurred. There is a decreased volume of aqueous layer (clear). Tube C and E indicate a wetting failure has occurred. There is an abnormal volume of Recovery Agent/Partitioning Oil (pink).</p>
<p>2.1 b</p> <p>After aspiration of Recovery Agent/ Partitioning Oil</p>	 <p>All liquid volumes are similar in the aqueous sample volume (clear) and residual Recovery Agent/Partitioning Oil (pink).</p>	 <p>Tube G indicates a reagent clog has occurred. There is a decreased volume of aqueous layer (clear). There is also a greater residual volume of Recovery Agent/Partitioning Oil (pink). Tube C and E indicate a wetting failure has occurred. There is an abnormal residual volume of Recovery Agent/Partitioning Oil (pink).</p>
<p>2.1 d</p> <p>After addition of Dynabeads Cleanup Mix</p>	 <p>All liquid volumes are similar after addition of the Dynabeads Cleanup Mix.</p>	 <p>Tube G indicates a reagent clog has occurred. There is an abnormal ratio of Dynabeads Cleanup Mix (brown) to Recovery Agent/Partitioning Oil (appears white). Tube C and E indicate a wetting failure has occurred. There is an abnormal ratio of Dynabeads Cleanup Mix (brown) to Recovery Agent/Partitioning Oil (appears white).</p>

If a channel clogs or wetting failure occurs during GEM generation, it is recommended that the sample be remade. If any of the listed issues occur, take a picture and send it to support@10xgenomics.com for further assistance.

Chromium Controller Errors

If the Chromium Controller or the Chromium Single Cell Controller fails to start, an error tone will sound and one of the following error messages will be displayed:

- a. **Chip not read – Try again:** Eject the tray, remove and/or reposition the Chromium Next GEM Secondary Holder assembly and try again. If the error message is still received after trying this more than twice, contact support@10xgenomics.com for further assistance.
- b. **Check gasket:** Eject the tray by pressing the eject button to check that the 10x Gasket is correctly installed on the Chromium Next GEM Chip. If the error message persists, contact support@10xgenomics.com for further assistance.
- c. **Error Detected: Row _ Pressure**
 - i. If this message is received within a few seconds of starting a run, eject the tray by pressing the eject button and check for dirt or deposits on the 10x Gasket. If dirt is observed, replace with a new 10x Gasket and try again. If the error message is still received after trying this more than twice, contact support@10xgenomics.com for further assistance.
 - ii. If this message is received after a few minutes into the run, the Chromium Next GEM Chip must be discarded. **Do not try running this Chromium Next GEM Chip again as this may damage the Chromium Controller.**
- d. **Invalid Chip CRC Value:** This indicates that a Chromium Next GEM Chip has been used with an older firmware version. The chip must be discarded. Contact support@10xgenomics.com for further assistance.

Appendix

Post Library Construction Quantification
Agilent TapeStation Traces
Oligonucleotide Sequences

10

Post Library Construction Quantification

- a. Thaw KAPA Library Quantification Kit for Illumina Platforms.
- b. Dilute **1 µl** sample with deionized water to appropriate dilutions that fall within the linear detection range of the KAPA Library Quantification Kit for Illumina Platforms. (For more accurate quantification, make the dilution(s) in duplicate).
- c. Make enough Quantification Master Mix for the DNA dilutions per sample and the DNA Standards (plus 10% excess) using the guidance for 1 reaction volume below.

Quantification Master Mix	1X (µl)
SYBR Fast Master Mix + Primer	12
Water	4
Total	16

- d. Dispense **16 µl** Quantification Master Mix for sample dilutions and DNA Standards into a 96 well PCR plate.
- e. Add **4 µl** sample dilutions and **4 µl** DNA Standards to appropriate wells. Centrifuge briefly.
- f. Incubate in a thermal cycler with the following protocol.

Step	Temperature	Run Time
1	95°C	00:03:00
2	95°C	00:00:05
3	67°C	00:00:30
4	Go to Step 2, 29X (Total 30 cycles)	

- g. Follow the manufacturer's recommendations for qPCR-based quantification. For library quantification for sequencer clustering, determine the concentration based on insert size derived from the Bioanalyzer/TapeStation trace.


Agilent TapeStation Traces

Agilent TapeStation Traces

Agilent TapeStation High Sensitivity D5000 ScreenTape[®] was used. Protocol steps correspond to the Chromium Next GEM Single Cell V(D)J Reagent Kits v1.1 User Guide with Feature Barcoding technology for Cell Surface Protein (CG000208).


Protocol Step 3.3 – cDNA QC & Quantification

Representative Trace

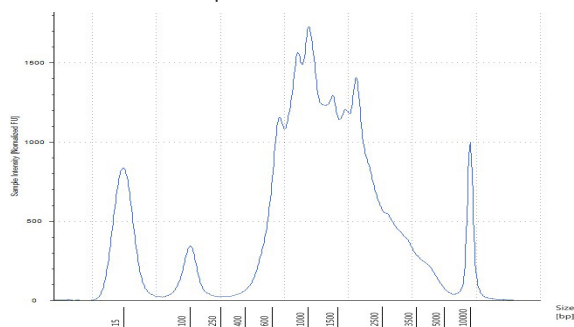


Protocol Step 6.7 – GEX Post Library Construction QC

Representative Trace

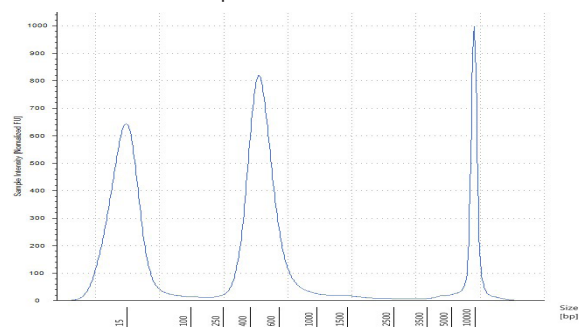


Protocol Step 5.6 – Post Library Construction QC (PBMCs enriched for TCR)

Representative Trace

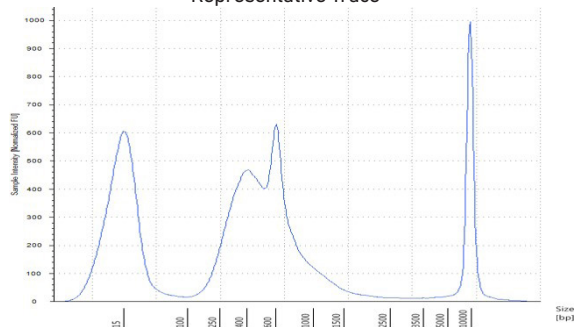


Protocol Step 7.3 – Post Library Construction QC

Representative Trace

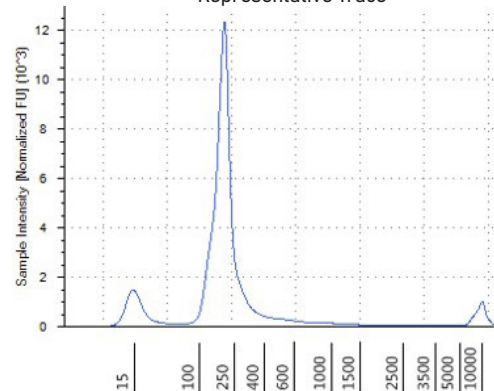

Protocol Step 5.6 – Post Library Construction QC (PBMCs enriched for Ig)

Representative Trace

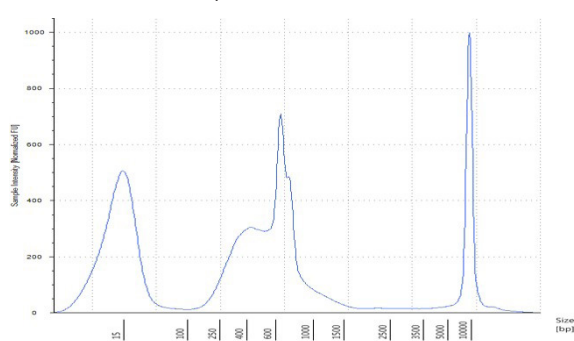

Protocol Step 1.5 – GEM-RT Incubation

Non-poly(dT) Poly(dT)VN
5'-AAGCAGTGGTATCAACGCAGAGTAC-TTTTTTTTTTTTTTTTTTTTTTTT-3'

3' **Capture Seq** **Feature Barcode** Read 2N

3'-AAAGAATATACCC-NNNNNNNNNN-NNNNNNNNNNNNNNNN-NNNNNNNNNN-GACAGAGAATATGTGTAGAGGC-5'

3' Read 1 Barcode 10x UMI TSO cDNA_Insert Poly(dT)VN Non-poly(dT) 5'

3'-GATGTGCTGCGAGAAGGCTAGA-NNNNNNNNNNNNNNNNNN-NNNNNNNNNN-AAAGAATATACCC-cDNA Insert-NVTTTTTTTTTTTTTTTTTTTTTTTTTTTTTTTT-CATGAGACGCAACTATGGTGACGAA-5'

Read 1 10x Barcode UMI Capture Seq Feature Barcode Read 2N

5'-CTACACGACGCTCTCCGATCT-NNNNNNNNNNNNNNNNNN-NNNNNNNNNN-TTTCTTATATGGG-NNNNNNNNNN-NNNNNNNNNNNNNNNNNN-NNNNNNNNNN-CTGTCTCTTATACATCTCCG-3'

3'-GATGTGCTGCGAGAAGGCTAGA-NNNNNNNNNNNNNNNN-NNNNNNNNNN-AAAGAATATACC-NNNNNNNNNN-NNNNNNNNNNNNNNNN-NNNNNNNNNN-GACAGAGAATATGTGTAGAGGC-5'

Protocol Step 3.1 – cDNA Amplification

Amplifies cDNA

Forward Primer: XXXXXXXXXX Partial Read 1
5'-CTACACGACGCTCTTCCGATCT-3'

Reverse Primer: Non-poly(dT)
5'-AAGCAGTGGTATCAACGCAGAG-3'

Amplifies DNA from cell surface protein Feature Barcode

Forward Primer: Partial Read 1
5'-CTACACGACGCTCTTCCGATCT-3'

Reverse Primer: Read 2N
5'-CTCGTGGGCTCGGAGATGTGTATAAGAGAC-3'

Amplified cDNA from poly-adenylated mRNA

Read 1 10x UMI TSO Poly-dT RT Primer

5'-CTACACGACGCTCTTCCGATCT-**NNNNNNNNNNNNNNNNNN**-**NNNNNNNNNN**-**TTTCTTATATGGG**-cDNA_Insert-**GTACTCTGCGTGTGATACCAC**TCGTT-3'
 3'-GATGTGCTGCGAGAAGGCTAGA-**NNNNNNNNNNNNNNNNNN**-**NNNNNNNNNN**-**AAAGAATATACCC**-cDNA_Insert-CATGAGACGCAACTATGGTGACGAA-5'









Amplified DNA from cell surface protein Feature Barcode

Read 1 10x UMI Capture Seq Feature Barcode Read 2N









5' -CTACACGACGCTCTCCGATCT-NNNNNNNNNNNNNNNN-NNNNNNNNNN-TTTCTTATATGGG-NNNNNNNNNN-NNNNNNNNNNNNNNNN-NNNNNNNNNN-CTGTCTCTTATACATCTCCGAGCCACAGG-3'

3' -GATGTGCTGCGAGAAGGCTAGA-NNNNNNNNNNNNNNNN-NNNNNNNNNN-AAAGAAATATACCC-NNNNNNNNNN-NNNNNNNNNNNNNNNN-NNNNNNNNNN-GACAGAGAATATGTGTAGAGGCTCGGTGCTC-5'

Protocol Step 4.1 – Target Enrichment 1

Human T Cell Mix 1 PN-2000008	Forward Primer: (final conc. 2 µM)  5'-AATGATACGGCGACCACCGA-GATCTACACTCTTCCCTACACGACGCTC-3'	Reverse Outer Primers: final conc. 1 µM each)  5'-TGAAGCGTTTGACATGCA-3' 5'-TCAGGCAGTATCTGGAGTCATTGAG-3'
Human B Cell Mix 1 PN-2000035	Forward Primer: (final conc. 1 µM)  5'-AATGATACGGCGACCACCGA-GATCTACACTCTTCCCTACACGACGCTC-3'	Reverse Outer Primers: (final conc. 0.5 µM each)  5'-CAGGGCACAGTCACATCCT-3' 5'-TGCTGGACCACGCATTGTGA-3' 5'-GGTTTGTGTCGACCCAGTCT-3' 5'-TTGTCCACCTTGGTGTGCT-3' 5'-CATGACGTCCTTGGAAAGGCA-3' 5'-TGTGGGACTTCCACTG-3' 5'-TTCTCGTAGTCTGCTTTGCTCAG-3'
Mouse T Cell Mix 1 PN-2000075	Forward Primer: (final conc. 2 µM)  5'-AATGATACGGCGACCACCGA-GATCTACACTCTTCCCTACACGACGCTC-3'	Reverse Outer Primers: (final conc. 0.5 µM each)  5'-CTGGTTGCTCCAGGCAATGG-3' 5'-TGATAGCCTGAGGGTCCGT-3'
Mouse B Cell Mix 1 PN-2000080	Forward Primer: (final conc. 1 µM)  5'-AATGATACGGCGACCACCGA-GATCTACACTCTTCCCTACACGACGCTC-3'	Reverse Outer Primers:  5'-TCAGCACGGGACAACTCTCT-3' (final conc. 0.375 µM) 5'-GCAGGAGACAGACTCTTCTCCA-3' (final conc. 0.175 µM) 5'-AACTGGCTGCTCATGGTGT-3' (final conc. 0.1 µM) 5'-TGGTGCAAGTGTGGTTGAGGT-3' (final conc. 0.3 µM) 5'-TGGTCACTTGGCTGGTGGTG-3' (final conc. 0.25 µM) 5'-CACTTGGCAGGTGAAGTCTTTCT-3' (final conc. 0.25 µM) 5'-AACCTTCAAGGATGCTCTTGGGA-3' (final conc. 0.3 µM) 5'-GGACAGGGATCCAGAGTTCCA-3' (final conc. 0.5 µM) 5'-AGGTGACGGTCTGACTTGGC-3' (final conc. 0.125 µM) 5'-GCTGGACAGGGCTCCATAGTT-3' (final conc. 0.125 µM) 5'-GGCACCTTGTCCAATCATGTTCC-3' (final conc. 0.250 µM) 5'-ATGTCGTTTCACTCGTCTTGGT-3' (final conc. 0.1 µM)

Protocol Step 4.3 – Target Enrichment 2

Human T Cell Mix 2 PN-2000009	Forward Primer: (final conc. 2 µM)  5'-AATGATACGGCGACCACCGA-GATCT-3'	Reverse Inner Primers: (final conc. 1 µM each)  5'-AGTCTCTCAGCTGGTACAGC-3' 5'-TCTGATGGCTCAAACACAGC-3'
Human B Cell Mix 2 PN-2000036	Forward Primer: (final conc. 1 µM)  5'-AATGATACGGCGACCACCGA-GATCT-3'	Reverse Inner Primers: (final conc. 0.5 µM each)  5'-GGGAAGTTTCTGGCGGTCA-3' 5'-GGTGGTACCCAGTTATCAAGCAT-3' 5'-GTGTCCAGGTCAACATCAC-3' 5'-TCCTGAGGACTGTAGGACAGC-3' 5'-CACGCTGCTCGTATCCGA-3' 5'-TAGCTGCTGGCCGC-3' 5'-GCGTTATCCACCTTCCACTGT-3'
Mouse T Cell Mix 2 PN-2000079	Forward Primer: (final conc. 0.5 µM)  5'-AATGATACGGCGACCACCGA-GATCT-3'	Reverse Inner Primers: (final conc. 0.5 µM each)  5'-AGTCAAAGTCGGTGAACAGGCA-3' 5'-GGCCAAGCACACGAGGGTA-3'
Mouse B Cell Mix 2 PN-2000081	Forward Primer: (final conc. 1 µM)  5'-AATGATACGGCGACCACCGA-GATCT-3'	Reverse Inner Primers:  5'-TACACACAGTGTGGCCTT-3' (final conc. 0.375 µM) 5'-CAGGCCACTGTACACCACT-3' (final conc. 0.175 µM) 5'-CAGGTCACATTATCGTGCCG-3' (final conc. 0.1 µM) 5'-GAGGCCAGCACAGTGACCT-3' (final conc. 0.3 µM) 5'-GCAGGGAAGTTCACAGTGCT-3' (final conc. 0.25 µM) 5'-CTGTTTGAGATCAGTTTGCCATCCT-3' (final conc. 0.25 µM) 5'-TGCGAGGTGGCTAGGTACTTG-3' (final conc. 0.3 µM) 5'-CCCTTGACCAAGCATCC-3' (final conc. 0.5 µM) 5'-AGGTCACGGAGGAACCAAGTTG-3' (final conc. 0.125 µM) 5'-GGCATCCCAAGTGTACCGA-3' (final conc. 0.125 µM) 5'-AGAAGATCCACTTCACTTGAAC-3' (final conc. 0.250 µM) 5'-GAAGCACAGACTGAGGCAC-3' (final conc. 0.1 µM)

Protocol Step 6.5 – Sample Index PCR (for 5' Gene Expression (GEX) Library Construction)

P7	Sample Index	Partial Read 2
5'-CAAGCAGAAGACGGCATACGAGAT	NNNNNNNN	-GTGACTGGAGTTCAGACGTGT-3'

The diagram illustrates the sequencing strategy for the 10x Genomics Chromium Single Cell 3' v2.1. It shows two reads, Read 1 and Read 2, each containing a P5 primer, a 10x Barcode, a UMI, and a TSO. An Insert is shown between the two reads. Read 2 also contains a Sample Index and a P7 primer.

5'-AATGATACGCGACCAACGA-GATCTACACTCTTTCCCTACAGACGCTCTTCOGATCT-NNNNNNNNNNNNNNNN-NNNNNNNNNN-TTCTTATATGGG-cDNA _ Insert-AGATCGGAAGAGCACAGTCGTGAACTCAGCTCAC-NNNNNNNN-ATCTGTGATCGCGCTCTTCGTGTTG-3'

3'-TTACTATCGCGCTGGTGCT-CTAGATGTGAGAAGGAGTGCTGCGAGGAGCTAGA-NNNNNNNNNNNNNNNN-NNNNNNNNNN-AAAGAATATACCC-cDNA _ Insert-TCTAGCCTTCTGTGTGACAGCTTGAGGTCAGTG-NNNNNNNN-TAGAGCATACCGCAGAAGCAAC-5'

Protocol Step 7.1 – Sample Index PCR (for Cell Surface Protein Library Construction)

P7	Sample Index N	Partial Read 2N
5'-CAAGCAGAAGACGGCATAACGAGAT-	NNNNNNNN	-GTCTCGTGGGCTCGG-3'

Diagram illustrating the 10x Genomics sequencing workflow. The workflow involves sequencing DNA molecules, capturing specific features, and indexing samples. The components shown are:

- P5
- Read 1
- 10x Barcode
- UMI
- Capture Seq
- Feature Barcode
- Read 2
- Sample Index
- P7

5'-AATGATACGGACCAACGA-GATCTACACTTTCCTCCACAGCGCTCTCCGATCT-**NNNNNNNNNNNNNNNN-NNNNNNNNNN-TTCTTATATGGG**-NNNNNNNNNN-**NNNNNNNNNNNNNNNNNNNN**-NNNNNNNNNN-CTGCTCTTATACACATCTCCGAGCCACAG-**NNNNNNNN-ACTCGTGATGCGGCTCTCTGCTG**-3'

3'-**TTTACTTGCCTGGTGCTG**-CTAGATGTGAAAGAGGATGTGCTCGAAGGCTAGA-**NNNNNNNNNNNNNNNN-NNNNNNNN-AAAGAATATACC**-NNNNNNNNNN-**NNNNNNNNNNNNNNNNNNNN**-NNNNNNNNNN-GACAGAGAATGTGTGATGAGGCTGGGTGCTC-**NNNNNNNN-TAGACATACGGCAGAGACGAC**-5'