USER GUIDE

Chromium Next GEM Single Cell 3' Reagent Kits v3.1 (Dual Index)

with Feature Barcode technology for CRISPR Screening and Cell Multiplexing



FOR USE WITH

Chromium Next GEM Single Cell 3' Kit v3.1, 16 rxns PN-1000268

Chromium Next GEM Single Cell 3' Kit v3.1, 4 rxns PN-1000269

3' Feature Barcode Kit, 16 rxns PN-1000262

3' CellPlex Kit Set A, 48 rxns PN-1000261

Chromium Next GEM Chip G Single Cell Kit, 48 rxns PN-1000120

Chromium Next GEM Chip G Single Cell Kit, 16 rxns PN-1000127

Dual Index Kit TT Set A, 96 rxns PN-1000215

Dual Index Kit NN Set A, 96 rxns PN-1000243

Dual Index Kit NT Set A, 96 rxns PN-1000242



Notices

Document Number

CG000389 • Rev A

Legal Notices

© 2021 10x Genomics, Inc. (10x Genomics). All rights reserved. Duplication and/or reproduction of all or any portion of this document without the express written consent of 10x Genomics, is strictly forbidden. Nothing contained herein shall constitute any warranty, express or implied, as to the performance of any products described herein. Any and all warranties applicable to any products are set forth in the applicable terms and conditions of sale accompanying the purchase of such product. 10x Genomics provides no warranty and hereby disclaims any and all warranties as to the use of any third-party products or protocols described herein. The use of products described herein is subject to certain restrictions as set forth in the applicable terms and conditions of sale accompanying the purchase of such product. A non-exhaustive list of 10x Genomics' marks, many of which are registered in the United States and other countries can be viewed at: www.10xgenomics.com/trademarks. 10x Genomics may refer to the products or services offered by other companies by their brand name or company name solely for clarity, and does not claim any rights in those third party marks or names. 10x Genomics products may be covered by one or more of the patents as indicated at: www.10xgenomics.com/patents. The use of products described herein is subject to 10x Genomics Terms and Conditions of Sale, available at www.10xgenomics.com/legal-notices, or such other terms that have been agreed to in writing between 10x Genomics and user. All products and services described herein are intended FOR RESEARCH USE ONLY and NOT FOR USE IN DIAGNOSTIC PROCEDURES.

Instrument & Licensed Software Updates Warranties

Updates to existing Instruments and Licensed Software may be required to enable customers to use new or existing products. In the event of an Instrument failure resulting from an update, such failed Instrument will be replaced or repaired in accordance with the 10x Limited Warranty, Assurance Plan or service agreement, only if such Instrument is covered by any of the foregoing at the time of such failure. Instruments not covered under a current 10x Limited Warranty, Assurance Plan or service agreement will not be replaced or repaired.

Support

Email: support@10xgenomics.com

10x Genomics

6230 Stoneridge Mall Road

Pleasanton, CA 94588 USA

Document Revision Summary

Document Number CG000389

Chromium Next GEM Single Cell 3' Reagent Kits v3.1

Title (Dual Index) with Feature Barcode technology for CRISPR

Screening and Cell Multiplexing User Guide

Revision Rev A

Revision Date March 2021

Table of Contents

Introduction	6
Chromium Next GEM Single Cell 3' Reagent Kits	7
10x Genomics Accessories	12
Recommended Thermal Cyclers	12
Additional Kits, Reagents & Equipment	13
Protocol Steps & Timing	15
Stepwise Objectives	16
CRISPR Screening Overview	21
Cell Multiplexing Oligo Labeling Guidelines	22
Tips & Best Practices	23
Step 1	31
GEM Generation & Barcoding	31
1.1 Prepare Master Mix	33
1.2 Load Chromium Next GEM Chip G	36
1.3 Run the Chromium Controller	37
1.4 Transfer GEMs	38
1.5 GEM-RT Incubation	38
Step 2	39
Post GEM-RT Cleanup & cDNA Amplification	39
2.1 Post GEM-RT Cleanup – Dynabeads	41
2.2 cDNA Amplification	43
2.3 cDNA Cleanup – SPRIselect	45
2.3A Pellet Cleanup (for 3' Gene Expression library)	45
2.3B Transferred Supernatant Cleanup (for Cell Multiplexing library)	46
2.3C Transferred Supernatant Cleanup (for CRISPR Screening library)	46
2.4 Post cDNA Amplification QC & Quantification	47
Step 3	48
3' Gene Expression Library Construction	48
3.0 3' Gene Expression Library Construction	49
3.1 Fragmentation, End Repair & A-tailing	51
3.2 Post Fragmentation, End Repair & A-tailing Double Sided Size Selection – SPRIselect	52
3.3 Adaptor Ligation	53
3.4 Post Ligation Cleanup – SPRIselect	54
3.5 Sample Index PCR	55

	TOC
3.6 Post Sample Index PCR Double Sided Size Selection – SPRIselect	56
3.7 Post Library Construction QC	57
Step 4	58
CRISPR Screening Library Construction	58
4.1 Guide RNA cDNA Cleanup – SPRIselect	60
4.2 Feature PCR	61
4.3 Post Feature PCR Cleanup – SPRIselect	62
4.4 Sample Index PCR	63
4.5 Post Sample Index PCR Double Sided Size Selection – SPRIselect	64
4.6 Post Library Construction QC	65
Step 5	66
Cell Multiplexing Library Construction	66
5.1 Sample Index PCR	68
5.2 Post Sample Index PCR Size Selection – SPRIselect	69
5.3 Post Library Construction QC	70
Sequencing	71
Troubleshooting	75
GEMs	76
Chromium Controller Errors	78
Appendix	79
Post Library Construction Quantification	80
Agilent TapeStation Traces	81
Agilent TapeStation Traces	82
LabChip Traces	83
Compatible sgRNA Specifications	84
Oligonucleotide Sequences	85
	87
	88

Introduction

Chromium Next GEM Single Cell 3' Reagent Kits v3.1 (Dual Index)

10x Genomics Accessories

Recommended Thermal Cyclers

Additional Kits, Reagents & Equipment

Protocol Steps & Timing

Stepwise Objectives


CRISPR Screening Guidelines

Cell Multiplexing Labeling Guidelines

Chromium Next GEM Single Cell 3' Reagent Kits

Chromium Next GEM Single Cell 3' Kit v3.1, 16 rxns PN-1000268

Chromium Next GEM Single Cell 3' GEM Kit v3.1 16 rxns PN-1000123 (store at -20°C)

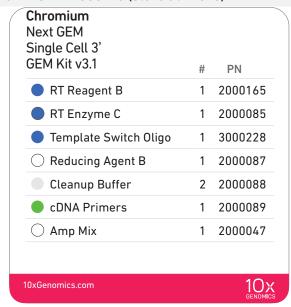


Library Construction Kit 16 rxns PN-1000190 (store at -20°C)



Chromium Next GEM Single Cell 3' Gel Bead Kit v3.1, 16 rxns PN-1000122 (store at -80°C)




Dynabeads™ MyOne™ SILANE PN-2000048 (store at 4°C)



Chromium Next GEM Single Cell 3' Kit v3.1, 4 rxns PN-1000269

Chromium Next GEM Single Cell 3' GEM Kit v3.1 4 rxns PN-1000130 (store at -20°C)

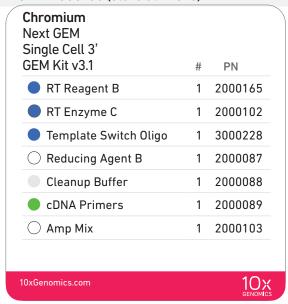

Library Construction Kit 4 rxns PN-1000196 (store at -20°C)




Chromium Next GEM Single Cell 3' Gel Bead Kit v3.1, 4 rxns PN-1000129 (store at -80°C)




Dynabeads™ MyOne™ SILANE PN-2000048 (store at 4°C)



3' Feature Barcode Kit, 16 rxns PN-1000262 (store at -20°C)

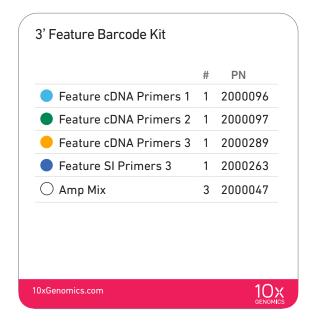

3' CellPlex Kit Set A, 48 rxns PN-1000261 (store at -20°C)

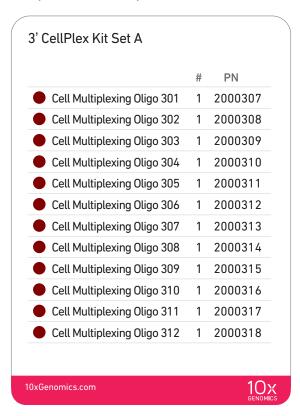

3' CellPlex Kit is used for labeling cells. Consult Demonstrated Protocol Cell Multiplexing Oligo Labeling for Single Cell RNA Sequencing Protocols with Feature Barcode technology (Document CG000391).

Dual Index Kit TT Set A, 96 rxns PN-1000215 (store at -20°C)




Dual Index Kit NN Set A, 96 rxns PN-1000243 (store at -20°C)



Dual Index Kit NT Set A, 96 rxns PN-1000242 (store at -20°C)



Chromium Next GEM Chip G Single Cell Kit, 48 rxns PN-1000120 (store at ambient temperature)

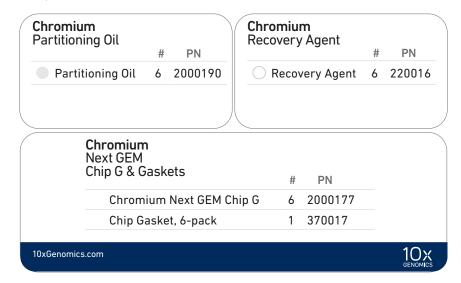

Chromium Next GEM Chip G Single Cell Kit, 16 rxns PN-1000127 (store at ambient temperature)



10x Genomics Accessories

Product	Part Number (Kit)	Part Number (Item)
10x Vortex Adapter	120251	330002
10x Magnetic Separator	120250	230003
Chromium Next GEM Secondary Holder	1000142	3000332

Recommended Thermal Cyclers

Thermal cyclers used must support uniform heating of $100 \mu l$ emulsion volumes.

Supplier	Description	Part Number
BioRad	C1000 Touch Thermal Cycler with 96-Deep Well Reaction Module	1851197
Eppendorf	MasterCycler Pro (discontinued)	North America 950030010 International 6321 000.019
Thermo Fisher Scientific	Veriti 96-Well Thermal Cycler	4375786

Additional Kits, Reagents & Equipment

The items in the table below have been validated by 10x Genomics and are highly recommended for the Single Cell 3' protocols. Substituting materials may adversely affect system performance. This list may not include some standard laboratory equipment.

Supplier	Description		Part Number (US)			
Plastics						
Eppendorf	PCR Tubes 0.2 ml 8-tube strips DNA LoBind Tubes, 1.5 ml DNA LoBind Tubes, 2.0 ml	DNA LoBind Tubes, 1.5 ml				
USA Scientific	TempAssure PCR 8-tube strip	Thermo Fisher Scientific PCR	1402-4700			
Thermo Fisher Scientific	MicroAmp 8-Tube Strip, 0.2 ml MicroAmp 8 -Cap Strip, clear	8-tube strips.	N8010580 N8010535			
Rainin	Tips LTS 200UL Filter RT-L200FLR Tips LTS 1ML Filter RT-L1000FLR Tips LTS 20UL Filter RT-L10FLR		30389240 30389213 30389226			
Kits & Reagents						
Thermo Fisher Scientific	Nuclease-free Water Low TE Buffer (10 mM Tris-HCl pH 8.0, 0.1 m	nM EDTA)	AM9937 12090-015			
Millipore Sigma	Ethanol, Pure (200 Proof, anhydrous)	Ethanol, Pure (200 Proof, anhydrous)				
Beckman Coulter	SPRIselect Reagent Kit	SPRIselect Reagent Kit				
Bio-Rad	10% Tween 20	10% Tween 20				
Ricca Chemical Company	Glycerin (glycerol), 50% (v/v) Aqueous Soluti	3290-32				
Qiagen	Qiagen Buffer EB		19086			
Equipment						
VWR	Vortex Mixer Divided Polystyrene Reservoirs VWR Mini Centrifuge (alternatively, use any equivalent mini centrif	fuge)	10153-838 41428-958 76269-066			
Eppendorf	Eppendorf ThermoMixer C Eppendorf SmartBlock 1.5 ml, Thermoblock (alternatively, use a temperature-controlled		5382000023 5360000038			
Rainin	Pipet-Lite Multi Pipette L8-50XLS+ Pipet-Lite Multi Pipette L8-200XLS+ Pipet-Lite Multi Pipette L8-10XLS+ Pipet-Lite Multi Pipette L8-20XLS+ Pipet-Lite LTS Pipette L-2XLS+ Pipet-Lite LTS Pipette L-10XLS+ Pipet-Lite LTS Pipette L-20XLS+ Pipet-Lite LTS Pipette L-100XLS+ Pipet-Lite LTS Pipette L-100XLS+ Pipet-Lite LTS Pipette L-200XLS+ Pipet-Lite LTS Pipette L-1000XLS+		17013804 17013805 17013802 17013803 17014393 17014388 17014392 17014384 17014391 17014382			

Additional Kits, Reagents & Equipment

The items in the table below have been validated by 10x Genomics and are highly recommended for the Single Cell 3' protocols. Substituting materials may adversely affect system performance. This list may not include some standard laboratory equipment.

Supplier	Description		Part Number (US)
Quantification & Quality Control			
Agilent	2100 Bioanalyzer Laptop Bundle High Sensitivity DNA Kit 4200 TapeStation High Sensitivity D1000 ScreenTape/Reagents High Sensitivity D5000 ScreenTape/Reagents	Choose Bioanalyzer, TapeStation, LabChip, Fragment Analyzer or Qubit	G2943CA 5067-4626 G2991AA 5067-5584/5067-5585 5067-5592/5067-5593
Thermo Fisher Scientific	Qubit 4.0 Flourometer Qubit dsDNA HS Assay Kit	based on availability & preference.	Q33238 Q32854
Advanced Analytical	Fragment Analyzer Automated CE System - 12 c Fragment Analyzer Automated CE System - 48/9 High Sensitivity NGS Fragment Analysis Kit	FSv2-CE2F FSv2-CE10F DNF-474	
PerkinElmer	LabChip GX Touch HT Nucleic Acid Analyzer DNA High Sensitivity Reagent Kit	CLS137031 CLS760672	
KAPA Biosystems	KAPA Library Quantification Kit for Illumina Plati	orms	KK4824

Protocol Steps & Timing

Day	Steps Steps	Timing Stop & Store
	Cell Preparation & Labeling	
1 h	Dependent on Cell Type	~1-2 h
	Step 1 – GEM Generation & Barcoding	
	 1.1 Prepare Reaction Mix 1.2 Load Chromium Next GEM Chip G 1.3 Run the Chromium Controller 1.4 Transfer GEMs 	20 min 10 min 18 min 3 min
4h	1.5 GEM-RT Incubation	55 min 4°C ≤72 h or −20°C ≤1 week
	Step 2 – Post GEM-RT Cleanup & cDNA Amplification	45 min
	2.1 Post GEM RT-Cleanup – Dynabead2.2 cDNA Amplification	40 min 5 ^{10P} 4°C ≤72 h or −20°C ≤1 week
6h	 2.3 cDNA Cleanup – SPRIselect 2.3A Pellet Cleanup 2.3B Transferred Supernatant Cleanup (Cell Multiplexing) 2.3C Transferred Supernatant Cleanup (CRISPR) 2.4 Screening) cDNA QC & Quantification 	15 min $4^{\circ}C \le 72 \text{ h or } -20^{\circ}C \le 4 \text{ weeks}$ 20 min $4^{\circ}C \le 72 \text{ h or } -20^{\circ}C \le 4 \text{ weeks}$ 20 min $4^{\circ}C \le 72 \text{ h or } -20^{\circ}C \le 4 \text{ weeks}$ 50 min
	Step 3 – 3' Gene Expression Library Construction	
	 3.1 Fragmentation, End Repair & A-tailing 3.2 Post Fragmentation, End Repair & A-tailing Double Sided Size Selection – SPRIselect 	45 min 30 min
	 3.3 Adaptor Ligation 3.4 Post Ligation Cleanup- SPRIselect 3.5 Sample Index PCR 3.6 Post Sample Index PCR Double Sided Size Selection- SPRIselect 3.6 Post Library Construction QC 	25 min 20 min 40 min 30 min 4°C ≤72 h 50 min
8h	Step 4 – CRISPR Screening Library Construction	
plus	 4.1 Guide RNA cDNA Cleanup 4.2 Feature PCR 4.3 Post Feature PCR Cleanup – SPRIselect 4.4 Sample Index PCR 4.5 Post Sample Index PCR Size Selection – SPRIselect 4.6 Post Library Construction QC 	20 min 50 min 20 min 30 min 20 min 4°C ≤72 h or -20°C long term 50 min
	Step 5 – Cell Multiplexing Library Construction	
	 5.1 Sample Index PCR 5.2 Post Sample Index PCR Size Selection- SPRIselect 5.3 Post Library Construction QC 	15 min 20 min 4°C ≤72 h or -20°C long term 50 min

Stepwise Objectives




The Chromium Single Cell Gene Expression Solution with Feature Barcode technology for CRISPR screening and cell multiplexing upgrades short read sequencers to deliver a scalable microfluidic platform for cell multiplexing while assessing CRISPR-mediated perturbations of gene expression by profiling 500-30,000 individual cells per sample. A pool of ~3,500,000 10x Barcodes are sampled separately to index each cell's transcriptome along with the CRISPR-mediated perturbations. It is done by partitioning thousands of cells into nanoliter-scale Gel Beads-in-emulsion (GEMs), where all generated DNA molecules share a common 10x Barcode. Libraries are generated and sequenced from the DNA molecules and 10x Barcodes are used to associate individual reads back to the individual partitions.

This document outlines the protocol for generating Single Cell 3' Gene Expression, CRISPR Screening, and Cell Multiplexing libraries from the same cells.

Single Cell 3' v3.1 Gel Beads


In addition to the poly(dT) primer that enables the production of barcoded, full-length cDNA from poly-adenylated mRNA, the Single Cell 3' v3.1 Gel Beads also include two additional primer sequences (Capture Sequence 1 and Capture Sequence 2), that enable capture and priming of Feature Barcode technology compatible targets or analytes of interest.

The poly(dT) primers along with one of the capture sequence primers are used in this protocol for generating Single Cell 3' Gene Expression, CRISPR Screening, and Cell Multiplexing libraries.

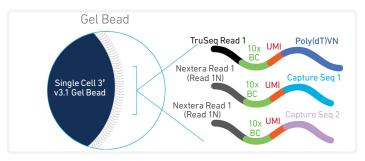

Step 1
GEM Generation &
Barcoding

GEMs are generated by combining barcoded Single Cell 3' v3.1 Gel Beads, a Master Mix with Cell Multiplexing Oligo labeled cells, and Partitioning Oil onto Chromium Chip G. To achieve single cell resolution, cells are delivered at a limiting dilution, such that the majority (\sim 90-99%) of generated GEMs contain no cell, while the remainder largely contain a single cell.

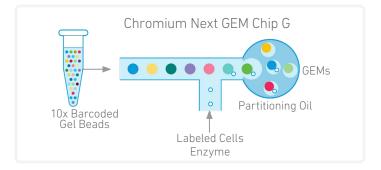

Step 1 GEM Generation & Barcoding

Immediately following GEM generation, the Gel Bead is dissolved releasing the three types of primers and any co-partitioned cell is lysed. The poly(dT) and one of the capture sequence primers in the gel bead are engaged simultaneously in two different reactions inside individual GEMs (primer with Capture Sequence 1 is not shown in the illustrated example).


A. Primers containing:

- an Illumina TruSeq Read 1 (read 1 sequencing primer)
- 16 nt 10x Barcode
- 12 nt unique molecular identifier (UMI)
- 30 nt poly(dT) sequence

B. Primers containing:

- an Illumina Nextera Read 1 (Read 1N; read 1 sequencing primer)
- 16 nt 10x Barcode
- 12 nt unique molecular identifier (UMI)
- Capture Sequence 1 or 2


Both are mixed with cell lysate and Master Mix containing RT reagents. Incubation of the GEMs produces barcoded, full-length cDNA from poly-adenylated mRNA from reagents in A and barcoded DNA from the sgRNA and Cell Multiplexing Oligo Feature Barcode from reagents in B.

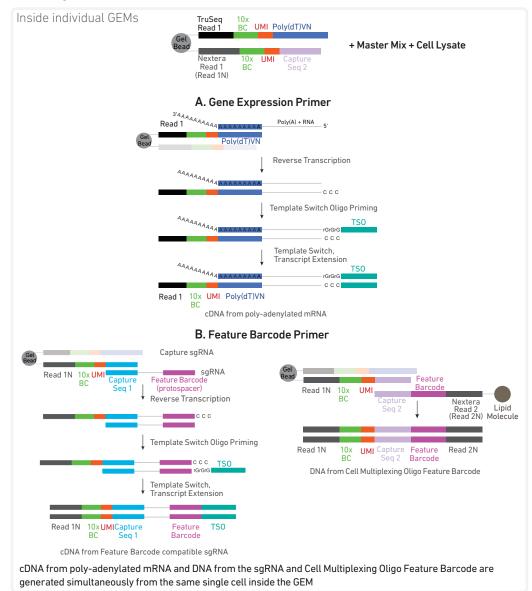

Step 2
Post GEM-RT Cleanup
& cDNA Amplification




After incubation, GEMs are broken and pooled fractions are recovered. Silane magnetic beads are used to purify the cell barcoded products from the post GEM-RT reaction mixture, which includes leftover biochemical reagents and primers. The cell barcoded cDNA molecules are amplified via PCR to generate sufficient mass for library constructions. Size selection is used to separate the amplified cDNA molecules for 3' Gene Expression, CRISPR Screening, and Cell Multiplexing library construction.

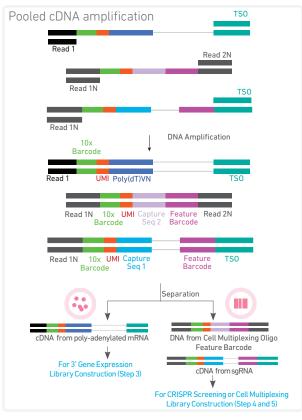

Step 3 3' Gene Expression Library Construction




Enzymatic fragmentation and size selection are used to optimize the cDNA amplicon size. P5, P7, i7 and i5 sample indexes, and TruSeq Read 2 (read 2 primer sequence) are added via End Repair, A-tailing, Adaptor Ligation, and PCR. The final libraries contain the P5 and P7 primers used in Illumina amplification.

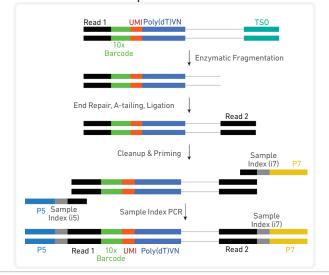

Step 4 CRISPR Screening Library Construction




Amplified cDNA from sgRNA molecules is used to generate CRISPR Screening libraries. P5, P7, i7 and i5 sample indexes, and TruSeq Read 2 (read 2 primer sequence) are added via PCR. The final libraries contain the P5 and P7 sequences necessary for amplification on the Illumina flow cell.

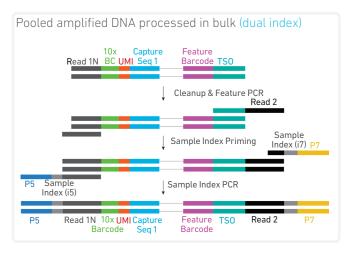

Step 5
Cell Multiplexing
Library Construction



Amplified DNA from Cell Multiplexing Oligo Feature Barcodes is used for library construction. P5, P7, i7 and i5 sample indexes, and Nextera Read 2 (read 2N primer sequence) are added via PCR. The final libraries contain the P5 and P7 sequences necessary for amplification on the Illumina flow cell.

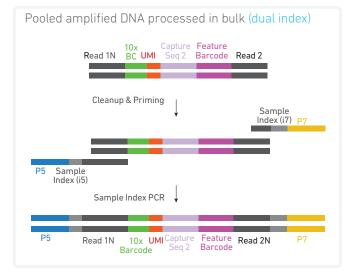

Step 6 Sequencing


The Single Cell 3' libraries comprise standard Illumina paired-end constructs which begin and end with P5 and P7. The 16 bp 10x Barcode and 12 bp UMI are encoded in Read 1. Read 2 is used to sequence the cDNA fragment in 3' Gene Expression libraries and the Feature Barcode (sgRNA protospacer) in the CRISPR Screening libraries. Read 2N is used to sequence the DNA from Cell Multiplexing Oligo Feature Barcode in the Cell Multiplexing libraries. i7 and i5 sample index sequences are incorporated as the sample index reads. Standard Illumina sequencing primer sites TruSeq Read 1 and TruSeq Read 2 in the 3' Gene Expression libraries, Nextera Read 1 and TruSeq Read 2 in the CRISPR Screening libraries, and Nextera Read 1 and Nextera Read 2 in the Cell Multiplexing libraries are used in paired-end sequencing.

Illumina sequencer compatibility, sample indices, library loading and pooling, recommended read depths and run parameters are summarized in step 6.

Chromium Single Cell 3' Gene Expression Dual Index Library




Chromium Single Cell 3' CRISPR Screening Dual Index Library



*Minimum required Read 2 length for CRISPR Screening libraries is 70 bp

Chromium Single Cell 3' Cell Multiplexing Dual Index Library




*Minimum required Read 2 length for Cell Multiplexing libraries is 15 bp

See Appendix for Oligonucleotide Sequences

CRISPR Screening Overview

The Chromium Single Cell Gene Expression Solution with Feature Barcode technology provides a high-throughput and scalable approach to obtain gene expression profiles along with perturbation phenotypes via direct capture of poly-adenylated mRNAs and single-guide RNAs (sgRNAs) from the same single cell (see Stepwise Objectives). For compatibility with Feature Barcode technology, sgRNAs should be engineered containing either Capture Sequence 1 or Capture Sequence 2. Two possible locations for integrating the capture sequence in the sgRNA include (1) within the sgRNA hairpin structure, or (2) immediately before the sgRNA termination signal, elongating the 3'-end of the sgRNA. However, alternate sgRNA integration locations for either of the two capture sequences may be possible depending on the specific application, type of construct used etc.

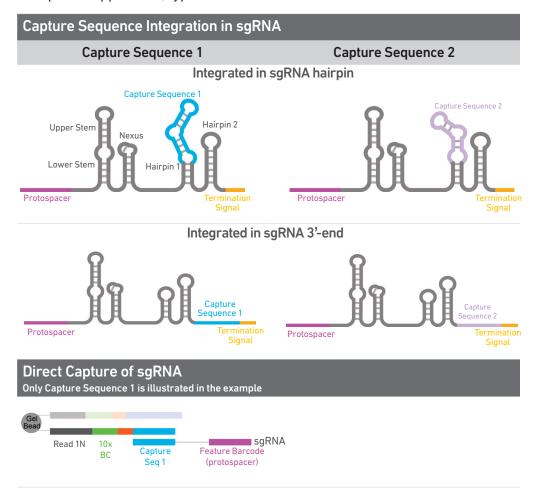




Performing sgRNA QC by qPCR, NGS, or other methods is recommended prior to proceeding with the Single Cell Gene Expression and CRISPR Screening Solution.

See Appendix for Compatible sqRNA Specifications

Cell Multiplexing Oligo Labeling Guidelines

Overview

The 10x Genomics 3' CellPlex Kit provides a species agnostic sample multiplexing solution through the use of a set of 12 Feature Barcode oligonucleotides each conjugated to a lipid. Individual cells or nuclei samples can be labeled with a Cell Multiplexing Oligo (CMO) and then pooled together prior to loading onto a 10x Genomics chip. The Feature Barcode molecules can be directly captured by the oligos present on the Gel Beads inside a GEM during GEM-RT and subsequently amplified (see Stepwise Objectives for assay scheme specifics). The amplified DNA generated from the Feature Barcode molecules can be used for Cell Multiplexing Library Construction. Upon sequencing and processing the data through Cell Ranger, pooled samples can be bioinformatically demultiplexed and analyzed as individual samples, with identified cell multiplets excluded.

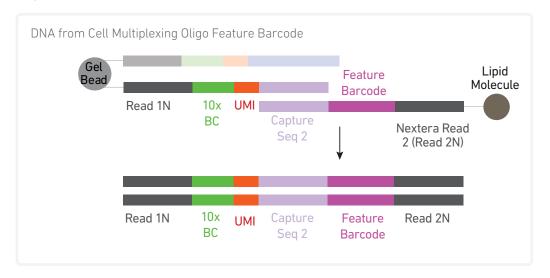

Demonstrated Protocols for Cell Multiplexing Oligo Labeling



For cell multiplexing oligo labeling guidance, consult Demonstrated Protocol Cell Multiplexing Oligo Labeling for Single Cell RNA Sequencing Protocols with Feature Barcode technology (Document CG000391).



Failure to label cells or nuclei with a Feature Barcode conjugated to the lipid molecule prior to using the cells for GEM Generation & Barcoding will preclude generation of a Cell Multiplexing library.

Tips & Best Practices



Icons











Emulsion-safe Plastics


• Use validated emulsion-safe plastic consumables when handling GEMs as some plastics can destabilize GEMs.

Cell Concentration

The optimal input cell concentration depends upon the desired cell recovery target.

Optimal Input Cell Concentration	Cell Recovery Target
700-1,200 cells/µl	500-10,000 cells
1,300-1,600 cells/µl	10,000-30,000 cells

- The presence of dead cells in the suspension may also reduce the recovery rate.
 Consult the 10x Genomics Single Cell Protocols Cell Preparation Guide and the Guidelines for Optimal Sample Preparation flowchart (Documents CG00053 and CG000126 respectively) for more information on preparing cells.
- Multiplets occur when more than one cell is partitioned into a single GEM. The
 multiplet rate increases linearly with increasing cell loads. When performing cell
 multiplexing, Cell Ranger can identify and filter multiplets if they contain cells
 labeled with different Cell Multiplexing Oligos (CMOs). For further details, consult the
 10x Genomics Cell Multiplexing Technical Note (CG000383).

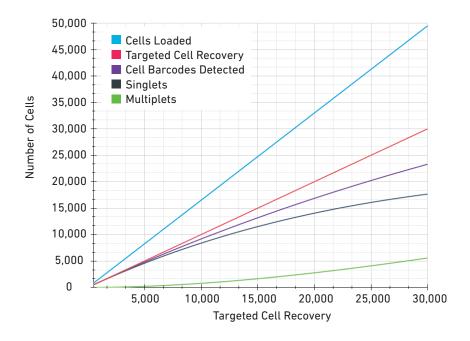

Cell Concentration

Targeted Cell Recovery	# of Cells Loaded	Cell Barcodes Detected	Singlets	Multiplets	Multiplet Rate (%)
500	825	~500	~500	~3	~0.4%
1,000	1,650	~1,000	~1,000	~10	~0.8%
2,000	3,300	~2,000	~2,000	~40	~1.6%
3,000	4,950	~3,000	~2,900	~80	~2.4%
4,000	6,600	~3,900	~3,800	~140	~3.2%
5,000	8,250	~4,800	~4,600	~210	~4.0%
6,000	9,900	~5,700	~5,400	~300	~4.8%
7,000	11,550	~6,600	~6,200	~400	~5.6%
8,000	13,200	~7,500	~7,000	~510	~6.4%
9,000	14,850	~8,400	~7,700	~640	~7.2%
10,000	16,500	~9,200	~8,400	~780	~8.0%
12,000	19,800	~10,900	~9,800	~1,100	~9.6%
14,000	23,100	~12,500	~11,000	~1,500	~11.2%
16,000	26,400	~14,000	~12,100	~1,900	~12.8%
18,000	29,700	~15,500	~13,100	~2,300	~14.4%
20,000	33,000	~16,900	~14,100	~2,800	~16.0%
22,000	36,300	~18,300	~15,000	~3,300	~17.6%
24,000	39,600	~19,600	~15,800	~3,900	~19.2%
26,000	42,900	~20,900	~16,500	~4,400	~20.8%
28,000	46,200	~22,200	~17,100	~5,000	~22.4%
30,000	49,500	~23,400	~17,700	~5,600	~24.0%

General Reagent Handling

- · Fully thaw and thoroughly mix reagents before use.
- Keep all enzymes and Master Mixes on ice during setup and use. Promptly move reagents back to the recommended storage.
- Calculate reagent volumes with 10% excess of 1 reaction values.
- Cover Partitioning Oil tubes and reservoirs to minimize evaporation.
- · If using multiple chips, use separate reagent reservoirs for each chip during loading.
- Thoroughly mix samples with the beads during bead-based cleanup steps.

50% Glycerol Solution

- Purchase 50% glycerol solution from Ricca Chemical Company, Glycerin (glycerol), 50% (v/v) Aqueous Solution, PN-3290-32.
- Prepare 50% glycerol solution:
 - i. Mix an equal volume of water and 99% Glycerol, Molecular Biology Grade.
 - ii. Filter through a 0.2 µm filter.
 - iii. Store at –20°C in 1-ml LoBind tubes. 50% glycerol solution should be equilibrated to room temperature before use.

Pipette Calibration

- Follow manufacturer's calibration and maintenance schedules.
- Pipette accuracy is particularly important when using SPRIselect reagents.

Chromium Next GEM Chip Handling



- Minimize exposure of reagents, chips, and gaskets to sources of particles and fibers, laboratory wipes, frequently opened flip-cap tubes, clothing that sheds fibers, and dusty surfaces.
- After removing the chip from the sealed bag, use in ≤ 24 h.
- Execute steps without pause or delay, unless indicated. When multiple chips are to be used, load, run, and collect the content from one chip before loading the next.
- Fill all unused input wells in rows labeled 1, 2, and 3 on a chip with an appropriate volume of 50% glycerol solution before loading the used wells. DO NOT add glycerol to the wells in the bottom NO FILL row.
- Avoid contacting the bottom surface of the chip with gloved hands and other surfaces.
 Frictional charging can lead to inadequate priming of the channels, potentially leading to either clogs or wetting failures.
- Minimize the distance that a loaded chip is moved to reach the Chromium Controller.
- Keep the chip horizontal to prevent wetting the gasket with oil, which depletes the input volume and may adversely affect the quality of the resulting emulsion.

Chromium Next GEM Secondary Holders



- Chromium Next GEM Secondary Holders encase Chromium Next GEM Chips.
- The holder lid flips over to become a stand, holding the chip at 45 degrees for optimal recovery well content removal.
- Squeeze the black sliders on the back side of the holder together to unlock the lid and return the holder to a flat position.



Chromium Next GEM Chip & Holder Assembly



- Align notch on the chip (upper left corner) and the holder.
- Insert the left-hand side of the chip under the guide. Depress the right-hand side of the chip until the spring-loaded clip engages.
- Close the lid before dispensing reagents into the wells.



Chromium Next GEM Chip Loading



- Place the assembled chip and holder flat on the bench with the lid closed.
- Dispense at the bottom of the wells without introducing bubbles.
- When dispensing Gel Beads into the chip, wait for the remainder to drain into the bottom of the pipette tips and dispense again to ensure complete transfer.
- Refer to Load Chromium Next GEM Chip G for specific instructions.



Gel Bead Handling



- Use one tube of Gel Beads per sample. DO NOT puncture the foil seals of tubes not used at the time.
- Equilibrate the Gel Beads strip to room temperature before use.
- Store unused Gel Beads at -80°C and avoid more than 12 freeze-thaw cycles. DO NOT store Gel Beads at -20°C.



- Snap the tube strip holder with the Gel Bead strip into a 10x Vortex Adapter. Vortex 30 sec.
- Centrifuge the Gel Bead strip for ~5 sec after removing from the holder. Confirm there are no bubbles at the bottom of the tubes and the liquid levels look even. Place the Gel Bead strip back in the holder and secure the holder lid.
- If the required volume of beads cannot be recovered, place the pipette tips against the sidewalls and slowly dispense the Gel Beads back into the tubes. DO NOT introduce bubbles into the tubes and verify that the pipette tips contain no leftover Gel Beads. Withdraw the full volume of beads again by pipetting slowly.

10x Gasket Attachment

- After reagents are loaded, attach the gasket by holding the tongue (curved end, to the right) and hook it on the left-hand tabs of the holder. Gently pull the gasket toward the right and hook it on the two right-hand tabs.
- DO NOT touch the smooth side of the gasket. DO NOT press down on the top of the gasket after attachment.
- Keep the assembly horizontal to avoid wetting the gasket with Partitioning Oil.




10x Magnetic Separator

- Offers two positions of the magnets (high and low) relative to a tube, depending on its orientation. Flip the magnetic separator over to switch between high (magnet•High) or low (magnet•Low) positions.
- If using MicroAmp 8-Tube Strips, use the high position (magnet•High) only throughout the protocol.



Magnetic Bead Cleanup Steps

- During magnetic bead based cleanup steps that specify waiting "until the solution clears", visually confirm clearing of solution before proceeding to the next step. See adjacent panel for an example.
- The time needed for the solution to clear may vary based on specific step, reagents, volume of reagents etc.

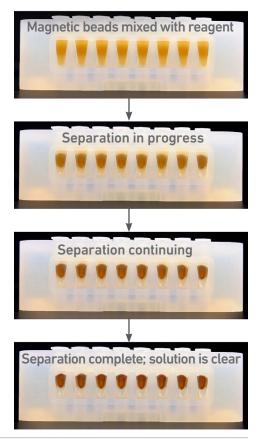


SPRIselect Cleanup & Size Selection

- After aspirating the desired volume of SPRIselect reagent, examine the pipette tips before dispensing to ensure the correct volume is transferred.
- Pipette mix thoroughly as insufficient mixing of sample and SPRIselect reagent will lead to inconsistent results.
- Use fresh preparations of 80% Ethanol.

Tutorial — SPRIselect Reagent: DNA Sample Ratios

SPRI beads selectively bind DNA according to the ratio of SPRIselect reagent (beads).

Example: Ratio = $\frac{\text{Volume of SPRIselect reagent added to the sample}}{\text{Volume of DNA sample}} = \frac{50 \, \mu l}{100 \, \mu l} = 0.5X$



After the first SPRI, supernatant is transferred for a second SPRI while larger fragments are discarded (green). After the second SPRI, fragments on beads are eluted and kept while smaller fragments are discarded (blue). Final sample has a tight fragment size distribution with reduced overall amount (black).

Tutorial — Double Sided Size Selection

Step a – First SPRIselect: Add 50 μl SPRIselect reagent to 100 μl sample (0.5X).

Ratio = $\frac{\text{Volume of SPRIselect reagent added to the sample}}{\text{Volume of DNA sample}} = \frac{50 \,\mu\text{l}}{100 \,\mu\text{l}} = 0.5X$

Step b - Second SPRIselect: Add 30 µl SPRIselect reagent to supernatant from step a (0.8X).

Ratio = $\frac{\text{Total Volume of SPRIselect reagent added to the sample (step a + b)}}{\text{Original Volume of DNA sample}} = \frac{50 \,\mu\text{l} + 30 \,\mu\text{l}}{100 \,\mu\text{l}} = 0.8X$

Enzymatic Fragmentation

 Ensure enzymatic fragmentation reactions are prepared on ice and then loaded into a thermal cycler pre-cooled to 4°C prior to initiating the Fragmentation, End Repair, and A-tailing incubation steps.

Sample Indices in Sample Index PCR

- Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run.
- Verify and use the specified index plate only. DO NOT use the plates interchangebaly.
- Each well in the Dual Index Plate contains a unique i7 and a unique i5 oligonucleotide.

Index Hopping Mitigation

Index hopping can impact pooled samples sequenced on Illumina sequencing platforms that utilize patterned flow cells and exclusion amplification chemistry. To minimize index hopping, follow the guidelines listed below.

- · Remove adapters during cleanup steps.
- Ensure no leftover primers and/or adapters are present when performing post-Library Construction QC.
- Store each library individually at 4°C for up to 72 h or at -20°C for long-term storage.
 DO NOT pool libraries during storage.
- Pool libraries prior to sequencing. An additional 1.0X SPRI may be performed for the pooled libraries to remove any free adapters before sequencing.
- Hopped indices can be computationally removed from the data generated from single cell dual index libraries.

Step 1

GEM Generation & Barcoding

- **1.1** Prepare Single Cell Master Mix
- 1.2 Load Chromium Next GEM Chip G
- **1.3** Run the Chromium Controller
- **1.4** Transfer GEMs
- **1.5** GEM-RT Incubation

1.0 GEM Generation & Barcoding

GET START	ED!								
Action		Item	10x PN	Preparation & Handling	Storage				
Equilibrate to Room Temperature		Single Cell 3' v3.1 Gel Beads	2000164	Equilibrate to room temperature 30 min before loading the chip.	-80°C				
		RT Reagent B	2000165	Vortex, verify no precipitate, centrifuge briefly.	-20°C				
	•	Template Switch Oligo	3000228	Centrifuge briefly, resuspend in 80 µl Low TE Buffer. Vortex 15 sec at maximum speed, centrifuge briefly, leave at room temperature for ≥ 30 min. After resuspension, store at -80°C.	−20°C				
	\bigcirc	Reducing Agent B	2000087	Vortex, verify no precipitate, centrifuge briefly.	-20°C				
Place on Ice	•	RT Enzyme C	2000085/ 2000102	Centrifuge briefly before adding to the mix.	-20°C				
A		Labeled Cell Suspension Consult Demonstrated Protocol Cell Multiplexing Oligo Labeling for Single Cell RNA Sequencing Protocols with Feature Barcode technology (CG000391)							
Obtain		Partitioning Oil	2000190	2000190 -					
		Chromium Next GEM Chip G	2000177	-	Ambient				
		10x Gasket	370017/ 3000072	See Tips & Best Practices.	Ambient				
		Chromium Next GEM Secondary Holder	3000332	See Tips & Best Practices.	Ambient				
		10x Vortex Adapter	330002	See Tips & Best Practices.	Ambient				
		50% glycerol solution	-	See Tips & Best Practices.	-				



Firmware Version 4.0 or higher is required in the Chromium Controller or the Chromium Single Cell Controller used for this Single Cell 3' v3.1 protocol.

If using <8 reactions

1.1 Prepare Master Mix



a. Prepare Master Mix on ice. Pipette mix 15x and centrifuge briefly.

Master Mix Add reagents in the order listed	PN	1Χ (μl)	4X + 10% (μl)	8X + 10% (µl)
RT Reagent B	2000165	18.8	82.7	165.4
Template Switch Oligo	3000228	2.4	10.6	21.1
Reducing Agent B	2000087	2.0	8.8	17.6
RT Enzyme C	2000085/ 2000102	8.7	38.3	76.6
Total	-	31.9	140.4	280.7

b. Add 31.9 µl Master Mix into each tube of a PCR 8-tube strip on ice.


Assemble Chromium Next GEM Chip G



After removing the chip from the sealed bag, use the chip in ≤ 24 h.



See Tips & Best Practices for chip handling instructions.



- Insert the left-hand side of the chip under the guide. Depress the righthand side of the chip until the springloaded clip engages.
- Close the lid before dispensing reagents into the wells.
- The assembled chip is ready for loading the indicated reagents. Refer to step 1.2 for reagent volumes and loading order.



Chromium Next GEM Chip G

Notch



For GEM generation, load the indicated reagents only in the specified rows, starting from row labeled 1, followed by rows labeled 2 and 3. DO NOT load reagents in the bottom row labeled NO FILL. See step 1.2 for details.



Step 1 GEM Generation & Barcoding



Cell Suspension Volume Calculator Table (Cell Recovery Target – 500-10,000)

(for step 1.2 of Chromium Next GEM Single Cell 3' v3.1 protocol)

Volume of Cell Suspension Stock per reaction (μl) | Volume of Nuclease-free Water per reaction (μl)



DO NOT add nuclease-free water directly to single cell suspension. Add nuclease-free water to the Master Mix. Refer to step 1.2b.

Cell Stock	to step i	.20.			Targeto	ed Cell Re	ecovery				
Concentration (Cells/µl)	500	1000	2000	3000	4000	5000	6000	7000	8000	9000	10000
100	8.3	16.5	33.0	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a
	35.0 4.1	26.7 8.3	10.2	24.8	33.0	41.3					
200	39.1	35.0	26.7	18.5	10.2	2.0	n/a	n/a	n/a	n/a	n/a
200	2.8	5.5	11.0	16.5	22.0	27.5	33.0	38.5	,	,	,
300	40.5	37.7	32.2	26.7	21.2	15.7	10.2	4.7	n/a	n/a	n/a
400	2.1	4.1	8.3	12.4	16.5	20.6	24.8	28.9	33.0	37.1	41.3
400	41.1	39.1	35.0	30.8	26.7	22.6	18.5	14.3	10.2	6.1	2.0
500	1.7	3.3	6.6	9.9	13.2	16.5	19.8	23.1	26.4	29.7	33.0
	41.6	39.9	36.6	33.3	30.0	26.7	23.4	20.1	16.8	13.5	10.2
600	1.4	2.8	5.5	8.3	11.0	13.8	16.5	19.3	22.0	24.8	27.5
	41.8 1.2	40.5 2.4	37.7 4.7	35.0 7.1	32.2 9.4	29.5 11.8	26.7 14.1	16.5	21.2	18.5 21.2	15.7 23.6
700	42.0	40.8	38.5	36.1	33.8	31.4	29.1	26.7	18.9 24.3	22.0	19.6
	1.0	2.1	4.1	6.2	8.3	10.3	12.4	14.4	16.5	18.6	20.6
800	42.2	41.1	39.1	37.0	35.0	32.9	30.8	28.8	26.7	24.6	22.6
222	0.9	1.8	3.7	5.5	7.3	9.2	11.0	12.8	14.7	16.5	18.3
900	42.3	41.4	39.5	37.7	35.9	34.0	32.2	30.4	28.5	26.7	24.9
1000	0.8	1.7	3.3	5.0	6.6	8.3	9.9	11.6	13.2	14.9	16.5
1000	42.4	41.6	39.9	38.3	36.6	35.0	33.3	31.7	30.0	28.4	26.7
1100	8.0	1.5	3.0	4.5	6.0	7.5	9.0	10.5	12.0	13.5	15.0
1100	42.5	41.7	40.2	38.7	37.2	35.7	34.2	32.7	31.2	29.7	28.2
1200	0.7	1.4	2.8	4.1	5.5	6.9	8.3	9.6	11.0	12.4	13.8
.=00	42.5	41.8	40.5	39.1	37.7	36.3	35.0	33.6	32.2	30.8	29.5
1300	0.6	1.3	2.5	3.8	5.1	6.3	7.6	8.9	10.2	11.4	12.7
	42.6	41.9	40.7	39.4	38.1	36.9	35.6	34.3	33.0	31.8	30.5
1400	0.6 42.6	1.2 42.0	2.4 40.8	3.5 39.7	4.7 38.5	5.9 37.3	7.1 36.1	8.3 35.0	9.4 33.8	10.6 32.6	11.8 31.4
	0.6	1.1	2.2	3.3	4.4	5.5	6.6	7.7	8.8	9.9	11.0
1500	42.7	42.1	41.0	39.9	38.8	37.7	36.6	35.5	34.4	33.3	32.2
	0.5	1.0	2.1	3.1	4.1	5.2	6.2	7.2	8.3	9.3	10.3
1600	42.7	42.2	41.1	40.1	39.1	38.0	37.0	36.0	35.0	33.9	32.9
1700	0.5	1.0	1.9	2.9	3.9	4.9	5.8	6.8	7.8	8.7	9.7
1700	42.7	42.2	41.3	40.3	39.3	38.3	37.4	36.4	35.4	34.5	33.5
1800	0.5	0.9	1.8	2.8	3.7	4.6	5.5	6.4	7.3	8.3	9.2
1000	42.7	42.3	41.4	40.5	39.5	38.6	37.7	36.8	35.9	35.0	34.0
1900	0.4	0.9	1.7	2.6	3.5	4.3	5.2	6.1	6.9	7.8	8.7
	42.8	42.3	41.5	40.6	39.7	38.9	38.0	37.1	36.3	35.4	34.5
2000	0.4	0.8	1.7	2.5	3.3	4.1	5.0	5.8	6.6	7.4	8.3
	42.8	42.4	41.6	40.7	39.9	39.1	38.3	37.4	36.6	35.8	35.0

Grey boxes: Volumes that would exceed the allowable water volume in each reaction Yellow boxes: Indicate a low transfer volume that may result in higher cell load variability

Blue boxes: Optimal range of cell stock concentration to maximize the likelihood of achieving the desired cell recovery target (500-10,000 cells)

Purple boxes: Optimal range of cell stock concentration to maximize the likelihood of achieving the desired cell recovery target (10,000-30,000 cells)



Cell Suspension Volume Calculator Table (Cell Recovery Target – 10,000-30,000)

(for step 1.2 of Chromium Next GEM Single Cell 3' v3.1 protocol)

Volume of Cell Suspension Stock per reaction (µl) | Volume of Nuclease-free Water per reaction (µl)



DO NOT add nuclease-free water directly to single cell suspension. Add nuclease-free water to the Master Mix. Refer to step 1.2b.

Cell Stock	Targeted Cell Recovery										
Concentration (Cells/µl)	10000	12000	14000	16000	18000	20000	22000	24000	26000	28000	30000
100	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a
200	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a
300	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a
400	41.3 2.0	n/a									
500	33.0 10.2	39.6 3.6	n/a								
600	27.5 15.7	33.0 10.2	38.5 4.7	n/a							
700	23.6 19.6	28.3 14.9	33.0 10.2	37.7 5.5	42.4 0.8	n/a	n/a	n/a	n/a	n/a	n/a
800	20.6 22.6	24.8 18.5	28.9 14.3	33.0 10.2	37.1 6.1	41.3 2.0	n/a	n/a	n/a	n/a	n/a
900	18.3 24.9	22.0 21.2	25.7 17.5	29.3 13.9	33.0 10.2	36.7 6.5	40.3 2.9	n/a	n/a	n/a	n/a
1000	16.5 26.7	19.8 23.4	23.1 20.1	26.4 16.8	29.7 13.5	33.0 10.2	36.3 6.9	39.6 3.6	n/a	n/a	n/a
1100	15.0 28.2	18.0 25.2	21.0 22.2	24.0 19.2	27.0 16.2	30.0 13.2	33.0 10.2	36.0 7.2	39.0 4.2	42.0 1.2	n/a
1200	13.8 29.5	16.5 26.7	19.3 24.0	22.0 21.2	24.8 18.5	27.5 15.7	30.3 13.0	33.0 10.2	35.8 7.5	38.5 4.7	41.3 2.0
1300	12.7 30.5	15.2 28.0	17.8 25.4	20.3 22.9	22.8 20.4	25.4 17.8	27.9 15.3	30.5 12.7	33.0 10.2	35.5 7.7	38.1 5.1
1400	11.8 31.4	14.1 29.1	16.5 26.7	18.9 24.3	21.2 22.0	23.6 19.6	25.9 17.3	28.3 14.9	30.6 12.6	33.0 10.2	35.4 7.8
1500	11.0 32.2	13.2 30.0	15.4 27.8	17.6 25.6	19.8 23.4	22.0 21.2	24.2 19.0	26.4 16.8	28.6 14.6	30.8 12.4	33.0 10.2
1600	10.3	12.4 30.8	14.4	16.5 26.7	18.6	20.6	22.7 20.5	24.8 18.5	26.8 16.4	28.9 14.3	30.9 12.3
1700	9.7	11.6	13.6	15.5 27.7	17.5 25.7	19.4	21.4	23.3	25.2 18.0	27.2 16.0	29.1 14.1
1800	9.2	11.0	12.8	14.7	16.5	18.3	20.2	22.0	23.8	25.7 17.5	27.5 15.7
1900	8.7	10.4	12.2	13.9	15.6	17.4	19.1	20.8	22.6	24.3	26.1
2000	8.3	9.9	31.0 11.6	13.2	27.6 14.9	25.8 16.5	18.2	19.8	20.6	23.1	17.1 24.8
Prov hovos:	35.0	33.3	31.7	30.0	28.4	26.7	25.1	23.4	21.8	20.1	18.5

Grey boxes: Volumes that would exceed the allowable water volume in each reaction
Yellow boxes: Indicate a low transfer volume that may result in higher cell load variability

Blue boxes: Optimal range of cell stock concentration to maximize the likelihood of achieving the desired cell recovery target (500-10,000 cells)

Purple boxes: Optimal range of cell stock concentration to maximize the likelihood of achieving the desired cell recovery target (10,000-30,000 cells)

1.2 Load Chromium Next GEM Chip G



After removing chip from the sealed bag, use in \leq 24 h. When loading the chip, raising and depressing the pipette plunger should each take \sim 5 sec.

When dispensing, raise the pipette tips at the same rate as the liquid is rising, keeping the tips slightly submerged.



a. Add 50% glycerol solution to each unused well

(if processing <8 samples/chip)

- 45 ul in each unused well in row labeled 3
- 50 µl in each unused well in row labeled 2
- 70 µl in each unused well in row labeled 1

A

DO NOT add 50% glycerol solution to the bottom row of NO FILL wells. DO NOT use any substitute for 50% glycerol solution.

b. Prepare Master Mix + Cell suspension

- Refer to the Cell Suspension Volume Calculator Table.
- Add the appropriate volume of nuclease-free water to Master Mix.
 Add corresponding volume of single cell suspension to Master Mix.
 Total of 75 μl in each tube.
- Gently pipette mix the cells suspension before adding to the Master Mix.

Cells Master Mix + Water

c. Load Row Labeled 1

- Gently pipette mix the Master Mix + Cell Suspension
- Using the same pipette tip, dispense 70 μl Master Mix + Cell Suspension into the bottom center of each well in row labeled 1 without introducing bubbles.

Master Mix + Sample

Glycerol



d. Prepare Gel Beads

- Snap the tube strip holder with the Gel Bead strip into a 10x Vortex Adapter.
 Vortex 30 sec.
- Centrifuge the Gel Bead strip for ~5 sec.
- Confirm there are no bubbles at the bottom of the tubes and the liquid levels are even.
- Place the Gel Bead strip back in the holder. Secure the holder lid.

Prep Gel Beads



e. Load Row Labeled 2

- · Puncture the foil seal of the Gel Bead tubes.
- Slowly aspirate **50 µl** Gel Beads.
- Dispense into the wells in row labeled 2 without introducing bubbles.
- Wait 30 sec.

Gel Beads



f. Load Row Labeled 3

 Dispense 45 μl Partitioning Oil into the wells in row labeled 3 from a reagent reservoir



Failure to add Partitioning Oil to the top row labeled 3 will prevent GEM generation and can damage the Chromium Controller.

Partitioning Oil



g. Attach GEM Gasket

- Align the notch with the top left-hand corner.
- Ensure the gasket holes are aligned with the wells.
- · Avoid touching the smooth surface.

A

Attach the gasket and run the chip in the Chromium Controller immediately after loading the Partitioning Oil.



1.3 Run the Chromium Controller



- **a.** Press the eject button on the Controller to eject the tray.
- b. Place the assembled chip with the gasket in the tray, ensuring that the chip stays horizontal. Press the button to retract the tray.
- **c.** Confirm the Chromium Chip G program on screen. Press the play button.



d. At completion of the run (~18 min), the Controller will chime. Immediately proceed to the next step.



Firmware Version 4.0 or higher is required in the Chromium Controller or the Chromium Single Cell Controller used for the Single Cell 3' v3.1 protocol.





1.4 Transfer GEMs



- a. Place a tube strip on ice.
- **b.** Press the eject button of the Controller and remove the chip.
- c. Discard the gasket. Open the chip holder. Fold the lid back until it clicks to expose the wells at 45 degrees.



- d. Check the volume in rows labeled 1-2. Abnormally high volume in any well indicates a clog.
- e. Slowly aspirate 100 μ l GEMs from the lowest points of the recovery wells in the top row labeled 3 without creating a seal between the tips and the bottom of the wells.



- f. Withdraw pipette tips from the wells. GEMs should appear opaque and uniform across all channels. Excess Partitioning Oil (clear) in the pipette tips indicates a potential clog.
- g. Over the course of ~20 sec, dispense GEMs into the tube strip on ice with the pipette tips against the sidewalls of the tubes.
- h. If multiple chips are run back-to-back, cap/ cover the GEM-containing tube strip and place on ice for no more than 1 h.

Expose Wells at 45 Degrees







1.5 GEM-RT Incubation

Use a thermal cycler that can accommodate at least 100 μ l volume. A volume of 125 μ l is the preferred setting on Bio-Rad C1000 Touch. In alternate thermal cyclers, use highest reaction volume setting.

a. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
53°C	125 μl	~55 min
Step	Temperature	Time
1	53°C	00:45:00
2	85°C	00:05:00
3	4°C	Hold



b. Store at 4°C for up to 72 h or at -20°C for up to a week, or proceed to the next step.

Step 2

Post GEM-RT Cleanup & cDNA Amplification

- **2.1** Post GEM-RT Cleanup Dynabeads
- 2.2 cDNA Amplification
- **2.3** cDNA Cleanup SPRIselect
- 2.4 cDNA QC & Quantification

2.0
Post GEM-RT Cleanup
& cDNA Amplification



GET STARTE	D!			
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room	Reducing Agent B	2000087	Thaw, vortex, verify no precipitate, centrifuge.	-20°C
Temperature	Feature cDNA Primers 3 Verify name & PN	2000289	Vortex, centrifuge briefly.	–20°C
	Dynabeads MyOne SILANE	2000048	Vortex thoroughly (≥30 sec) immediately before adding to the mix.	4°C
	Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
	Agilent Bioanalyzer High Sensitivity Kit If used for QC and quantification	-	Manufacturer's recommendations.	-
	Agilent TapeStation ScreenTape and Reagents If used for QC and quantification	-	Manufacturer's recommendations.	-
	Qubit dsDNA HS Assay Kit If used for QC and quantification	-	Manufacturer's recommendations.	-
Place on ice	○ Amp Mix	2000047/ 2000103	Vortex, centrifuge briefly.	-20°C
Thaw at 65°C	Cleanup Buffer	2000088	Thaw for 10 min at 65°C at max speed on a thermomixer. Verify no visible crystals. Cool to room temperature.	-20°C
Obtain	Recovery Agent	220016	-	Ambient
	Qiagen Buffer EB	-	Manufacturer's recommendations.	-
	Bio-Rad 10% Tween 20	-	Manufacturer's recommendations.	-
	10x Magnetic Separator	230003	-	Ambient
	Prepare 80% Ethanol Prepare 15 ml for 8 reactions.	-	-	-

2.1 Post GEM-RT Cleanup – Dynabeads



a. Add 125 µl Recovery Agent to each sample at room temperature. DO NOT pipette mix or vortex the biphasic mixture. Wait 2 min.

The resulting biphasic mixture contains Recovery Agent/Partitioning Oil (pink) and aqueous phase (clear), with no persisting emulsion (opaque).



If biphasic separation is incomplete:

Firmly secure the cap on the tube strip, ensuring that no liquid is trapped between the cap and the tube rim. Mix by inverting the capped tube strip 5x, centrifuge briefly, and proceed to step b. DO NOT invert without firmly securing the caps.



A smaller aqueous phase volume indicates a clog during GEM generation.



b. Slowly remove and discard 125 µl Recovery Agent/Partitioning Oil (pink) from the bottom of the tube. DO NOT aspirate any aqueous sample.

Remove Recovery Agent

c. Prepare Dynabeads Cleanup Mix.

	Dynabeads Cleanup Mix Add reagents in the order listed	PN	1X (μl)	4X + 10% (μl)	8X + 10% (μl)
	Cleanup Buffer	2000088	182	801	1602
Resuspend clump	Dynabeads MyOne SILANE Vortex thoroughly (≥30 sec) immediately before adding to the mix. Aspirate the full liquid volume with a pipette tip to verify that the beads have not settled in the bottom of the tube. If clumps are present, pipette mix to resuspend completely. DO NOT centrifuge before use.	2000048	8	35	70
	Reducing Agent B	2000087	5	22	44
	Nuclease-free Water		5	22	44
	Total	-	200	880	1760



- **d.** Vortex and add **200 μl** to each sample. Pipette mix 10x (pipette set to 200 μl).
- e. Incubate 10 min at room temperature (keep caps open). Pipette mix again at ~5 min after start of incubation to resuspend settled beads.





f. Prepare Elution Solution I. Vortex and centrifuge briefly.

Elution Solution I Add reagents in the order listed	PN	1X (μl)	10Χ (μl)
Buffer EB	-	98	980
10% Tween 20	-	1	10
Reducing Agent B	2000087	1	10
Total	-	100	1000



g. At the end of 10 min incubation, place on a 10x Magnetic Separator•High position (magnet•High) until the solution clears.

A white interface between the aqueous phase and Recovery Agent is normal.

- h. Remove the supernatant (aqueous phase and Recovery Agent).
- i. Add 300 µl 80% ethanol to the pellet while on the magnet. Wait 30 sec.
- j. Remove the ethanol.
- k. Add 200 µl 80% ethanol to pellet. Wait 30 sec.
- I. Remove the ethanol.
- m.Centrifuge briefly. Place on the magnet-Low.
- n. Remove remaining ethanol. Air dry for 1 min.
- o. Remove from the magnet. Immediately add 35.5 µl Elution Solution I.
- **p.** Pipette mix (pipette set to 30 μ l) without introducing bubbles.
- q. Incubate 2 min at room temperature.
- r. Place on the magnet•Low until the solution clears.
- **s.** Transfer $35 \mu l$ sample to a new tube strip.

2.2 cDNA Amplification





a. Prepare cDNA Amplification Mix on ice. Vortex and centrifuge briefly.

cDNA Amplification Reaction Mix Add reagents in the order listed	PN	1Χ (μl)	4X + 10% (μl)	8X + 10% (μl)
) Amp Mix	2000047	50	220	440
Feature cDNA Primers 3				
Verify name & PN Use indicated primer only	2000289	15	66	132
Total	-	65	286	572

- b. Add 65 µl cDNA Amplification Reaction Mix to 35 µl sample.
- c. Pipette mix 15x (pipette set to 90 μ l). Centrifuge briefly.
- **d.** Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~30-45 min
Step	Temperature	Time
1	98°C	00:03:00
2	98°C	00:00:15
3	63°C	00:00:20
4	72°C	00:01:00
5	Go to Step 2, see table	e below for total # of cycles
6	72°C	00:01:00
7	4°C	Hold

The optimal number of cycles is a trade-off between generating sufficient final mass for library construction and minimizing PCR amplification artifacts. The number of cDNA cycles should also be reduced if large numbers of cells are sampled.


Recommended starting point for cycle number optimization.


Targeted Cell Recovery	Total Cycles
<500	13
500-6,000	12
6,000-30,000	11



e. Store at 4° C for up to 72 h or -20° C for ≤ 1 week, or proceed to the next step.

Step Overview (steps 2.2 & 2.3)

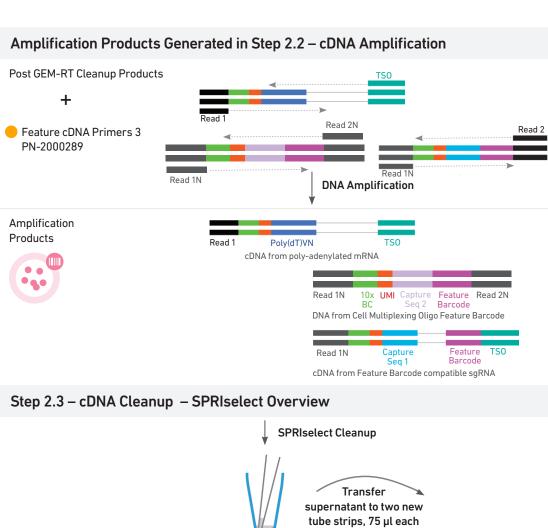

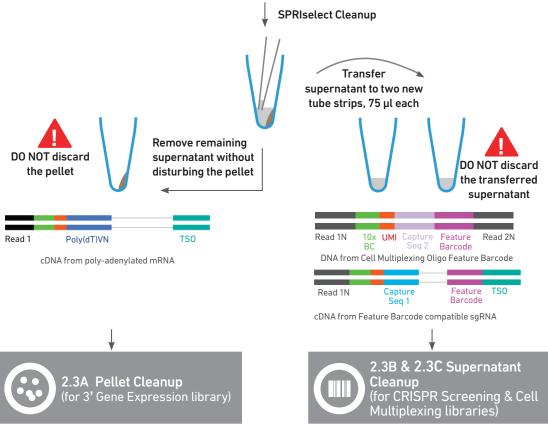

Step 2 cDNA Amplification & QC

2.3 cDNA Cleanup – SPRIselect

a. Vortex to resuspend the SPRIselect reagent. Add 60 μ l SPRIselect reagent (0.6X) to each sample and pipette mix 15x (pipette set to 150 μ l).

- **b.** Incubate **5 min** at **room temperature**.
- c. Place on the magnet•High until the solution clears.



- d. Transfer and save 75 μl supernatant each into two new tube strips without disturbing the pellet. Maintain at room temperature. DO NOT discard the transferred supernatant (cleanup for CRISPR Screening and Cell Multiplexing library construction).
- e. Remove the remaining supernatant from the pellet without disturbing the pellet. DO NOT discard the pellet (cleanup for 3' Gene Expression library construction). Immediately proceed to Pellet Cleanup (step 2.3A).



2.3A Pellet Cleanup (for 3' Gene Expression library)

- i. Add 200 µl 80% ethanol to the pellet. Wait 30 sec.
- ii. Remove the ethanol.
- iii. Repeat steps i and ii for a total of 2 washes.
- iv. Centrifuge briefly and place on the magnet-Low.
- v. Remove any remaining ethanol. Air dry for 2 min. DO NOT exceed 2 min as this will decrease elution efficiency.
- vi. Remove from the magnet. Add 40.5 μ l Buffer EB. Pipette mix 15x (pipette set to 35 μ l).
- vii. Incubate 2 min at room temperature.
- viii. Place the tube strip on the magnet. High until the solution clears.
- ix. Transfer 40 µl sample to a new tube strip.
- Store at 4°C for up to 72 h or at -20°C for up to 4 weeks, or proceed to step 2.4 followed by step 3 for 3' Gene Expression Library Construction.



Proceed immediately to next page for supernatant cleanup.

Step 2 cDNA Amplification & QC

2.3 cDNA Cleanup – SPRIselect



2.3B Transferred Supernatant Cleanup (for Cell Multiplexing library)

- i. Vortex to resuspend the SPRIselect reagent. Add **70** μ l SPRIselect reagent **(2.0X)** to **75** μ l of the transferred supernatant and pipette mix 15x (pipette set to 130 μ l).
- ii. Incubate for 5 min at room temperature.
- iii. Place on the magnet•High until the solution clears.
- iv. Remove supernatant.
- v. Add 300 µl 80% ethanol to the pellet. Wait 30 sec.
- vi. Remove the ethanol.
- vii. Repeat steps v and vi for a total of 2 washes.
- viii. Centrifuge briefly and place on the magnet Low.
- ix. Remove any remaining ethanol. Air dry for 2 min. DO NOT exceed 2 min as this will decrease elution efficiency.
- x. Remove from the magnet. Add 40.5 µl Buffer EB. Pipette mix 15x (pipette set to 35 µl).
- xi. Incubate 2 min at room temperature.
- xii. Place the tube strip on the magnet•High until the solution clears.
- xiii. Transfer 40 µl sample to a new tube strip.
- Store at 4°C for up to 72 h or at -20°C for up to 4 weeks, or proceed directly to step 5 for Cell Multiplexing Library Construction.



2.3C Transferred Supernatant Cleanup (for CRISPR Screening library)

- i. Vortex to resuspend the SPRIselect reagent. Add 30 μ l SPRIselect reagent (1.2X) to 75 μ l of the transferred supernatant and pipette mix 15x (pipette set to 80 μ l).
- ii. Incubate for 5 min at room temperature.
- iii. Place on the magnet•High until the solution clears.
- iv. Remove supernatant.
- v. Add 300 µl 80% ethanol to the pellet. Wait 30 sec.
- vi. Remove the ethanol.
- vii. Repeat steps v and vi for a total of 2 washes.
- viii. Centrifuge briefly and place on the magnet•Low.
- ix. Remove any remaining ethanol. Air dry for 2 min. DO NOT exceed 2 min as this will decrease elution efficiency.
- x. Remove from the magnet. Add 40.5 μl Buffer EB. Pipette mix 15x (pipette set to 35 μl).
- xi. Incubate 2 min at room temperature.
- xii. Place the tube strip on the magnet•High until the solution clears.
- xiii. Transfer 40 µl sample to a new tube strip.
- Store at 4°C for up to 72 h or at -20°C for up to 4 weeks, or proceed directly to step 4 for CRISPR Screening Library Construction.


Step 2 cDNA Amplification & QC

2.4 Post cDNA Amplification QC & Quantification

a. Run 1 μl of sample from Pellet Cleanup (step 2.3A-x), diluted 1:10 on an Agilent Bioanalyzer High Sensitivity chip. DO NOT run sample from 2.3B and 2.3C Transferred Supernatant Cleanup step.

For input cells with low RNA content (<1pg total RNA/cell), 1 µl undiluted product may be run.


Lower molecular weight product (35 – 150 bp) may be present. This is normal and does not affect sequencing or application performance.

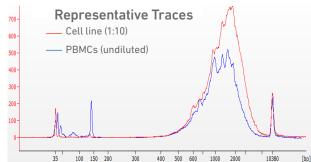


EXAMPLE CALCULATION

i. Select Region

Under the "Electropherogram" view choose the "Region Table". Manually select the region of $\sim 200 - 9000$ bp



ii. Note Concentration [pg/µl]



iii. Calculate

Multiply the cDNA concentration [pg/ μ l] reported via the Agilent 2100 Expert Software by the elution volume (40 μ l) of the Post cDNA Amplification Reaction Clean Up sample (taking any dilution factors into account) and then divide by 1000 to obtain the total cDNA yield in ng.

Example Calculation of cDNA Total Yield

Concentration: 1890.19 pg/µl Elution Volume: 40

Dilution Factor: 10

Total cDNA Yield

- = Conc'n (pg/μl) x Elution Volume x Dilution Factor 1000 (pg/ng)
- = $\frac{1890.19 (pg/\mu l) \times 40 \times 10}{1000 (pg/ng)}$ = 756.08 ng



Carry forward **ONLY 25**% of total cDNA yield into 3' Gene Expression Library Construction (step 3)

- = 0.25 x Total cDNA yield
- = 0.25 x 756.08= 189.02 ng

Refer to step 3.5 for appropriate number of Sample Index PCR cycles based on carry forward cDNA yield/input cDNA.

Alternate Quantification Methods See Appendix for representative traces

- Agilent TapeStation
- LabChip
- Fragment Analyzer

Agilent Bioanalyzer, Agilent TapeStation, LabChip, and Fragment Analyzer are the recommended methods for accurate quantification. If using Qubit Fluorometer and Qubit dsDNA HS Assay Kit, see Appendix.

Step 3

3' Gene Expression Library Construction

- 3.1 Fragmentation, End Repair & A-tailing
- 3.2 Post Fragmentation End Repair & A-tailing Double Sided Size Selection SPRIselect
- **3.3** Adaptor Ligation
- **3.4** Post Ligation Cleanup SPRIselect
- 3.5 Sample Index PCR
- 3.6 Post Sample Index PCR Double Sided Size Selection SPRIselect
- **3.7** Post Library Construction QC

3.0 3' Gene Expression Library Construction




GET START	ED!				
Action		Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	•	Fragmentation Buffer	2000091	Vortex, verify no precipitate, centrifuge briefly.	–20°C
remperature		Adaptor Oligos	2000094	Vortex, centrifuge briefly.	-20°C
		Ligation Buffer	2000092	Vortex, verify no precipitate, centrifuge briefly.	–20°C
DUAL		Dual Index Plate TT Set A Verify name & PN Use indicated plate only	3000431	-	-20°C
		Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
		Agilent TapeStation Screen Tape and Reagents If used for QC	-	Manufacturer's recommendations.	-
		Agilent Bioanalyzer High Sensitivity kit If used for QC	-	Manufacturer's recommendations.	-
		DNA High Sensitivity Reagent Kit If LabChip used for QC	-	Manufacturer's recommendations.	-
Place on Ice	•	Fragmentation Enzyme	2000090/ 2000104	Centrifuge briefly.	-20°C
		DNA Ligase	220110/ 220131	Centrifuge briefly.	-20°C
		Amp Mix	2000047/ 2000103	Centrifuge briefly.	-20°C
		KAPA Library Quantification Kit for Illumina Platforms	-	Manufacturer's recommendations.	-
Obtain	(Qiagen Buffer EB	-	-	Ambient
	1	10x Magnetic Separator	230003	See Tips & Best Practices.	Ambient
	F	Prepare 80% Ethanol Prepare 20 ml for 8 eactions	-	Prepare fresh.	Ambient

Step Overview (Step 3.1d)

Correlation between input & library complexity

A Single Cell 3' Gene Expression library is generated using a fixed proportion (10 μ l, 25%) of the total cDNA (40 μ l) obtained at step 2.3A-ix. The complexity of this library will be comparable to one generated using a higher proportion (>25%) of the cDNA. The remaining proportion (30 μ l, 75%) of the cDNA may be stored at 4°C for up to 72 h or at -20°C for longer-term storage (up to 4 weeks).

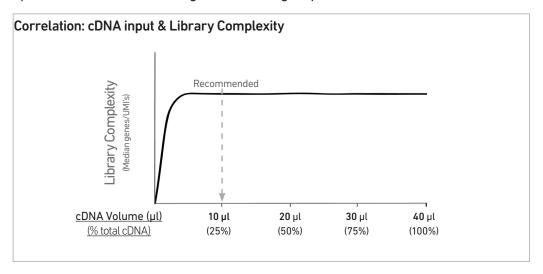

Note that irrespective of the total cDNA yield (ng), which may vary based on cell type, targeted cell recovery etc., this protocol has been optimized for a broad range of input mass (ng), as shown in the example below. The total number of SI PCR cycles (step 3.5e) should be optimized based on carrying forward a fixed proportion (10 μ l, 25%) of the total cDNA yield calculated during Post cDNA Amplification QC & Quantification (step 2.4).

Example: Library Construction Input Mass & SI PCR Cycles					
Cell Type	Targeted	Total cDNA Yield –	cDNA Input into Fragmentation		SI PCR Cycle
Cett Type	Cell Recovery	(ng)	Volume (μl)	Mass (ng)	Number
High RNA Content	Low 6	250 ng	10 μl	62.5 ng	13
	High	1900 ng	10 μl	475 ng	10
Low RNA Content	Low	1 ng	10 μl	0.25 ng	16
	High	200 ng	10 μl	50 ng	12

3.1
Fragmentation,
End Repair & A-tailing

a. Prepare a thermal cycler with the following incubation protocol.

Lid Temperature	Reaction Volume	Run Time
65°C	50 μl	~35 min
Step	Temperature	Time
Pre-cool block Pre-cool block prior to preparing the Fragmentation Mix	4°C	Hold
Fragmentation	32°C	00:05:00
End Repair & A-tailing	65°C	00:30:00
Hold	4°C	Hold



- b. Vortex Fragmentation Buffer. Verify there is no precipitate.
- c. Prepare Fragmentation Mix on ice. Pipette mix and centrifuge briefly.

Fragmentation Mix Add reagents in the order listed	PN	1X (μl)	4Χ + 10% (μl)	8X + 10% (µl)
Fragmentation Buffer	2000091	5	22	44
Fragmentation Enzyme	2000090/ 2000104	10	44	88
Total	-	15	66	132

d. Transfer ONLY 10 μ l purified cDNA sample from Pellet Cleanup (step 2.3A-x) to a tube strip.

Note that only 10 μ l (25%) cDNA sample transfer is sufficient for generating 3' Gene Expression library.

The remaining 30 μ l (75%) cDNA sample can be stored at 4°C for up to 72 h or at -20°C for up to 4 weeks for generating additional 3' Gene Expression libraries.

- e. Add 25 µl Buffer EB to each sample.
- f. Add 15 µl Fragmentation Mix to each sample.
- g. Pipette mix 15x (pipette set to 35 μ l) on ice. Centrifuge briefly.
- **h.** Transfer into the pre-cooled thermal cycler (4°C) and press "SKIP" to initiate the protocol.

3.2 Post Fragmentation, End Repair & A-tailing Double Sided Size Selection – SPRIselect

- a. Vortex to resuspend SPRIselect reagent. Add **30 µl** SPRIselect **(0.6X)** reagent to each sample. Pipette mix 15x (pipette set to 75 µl).
- b. Incubate 5 min at room temperature.
- c. Place on the magnet•High until the solution clears. DO NOT discard supernatant.





- **d.** Transfer **75** μ**l** supernatant to a new tube strip.
- e. Vortex to resuspend SPRIselect reagent. Add 10 μl SPRIselect reagent (0.8X) to each sample. Pipette mix 15x (pipette set to 80 μl).
- f. Incubate 5 min at room temperature.
- g. Place on the magnet•High until the solution clears.





- h. Remove 80 μl supernatant. DO NOT discard any beads.
- i. Add 125 µl 80% ethanol to the pellet. Wait 30 sec.
- j. Remove the ethanol.
- k. Repeat steps i and j for a total of 2 washes.
- Centrifuge briefly. Place on the magnet•Low until the solution clears. Remove remaining ethanol. DO NOT over dry to ensure maximum elution efficiency.
- **m.** Remove from the magnet. Add **50.5** μ l Buffer EB to each sample. Pipette mix 15x (pipette set to 45 μ l).
- n. Incubate 2 min at room temperature.
- o. Place on the magnet. High until the solution clears.
- **p.** Transfer $50 \mu l$ sample to a new tube strip.

3.3 Adaptor Ligation

a. Prepare Adaptor Ligation Mix. Pipette mix and centrifuge briefly.

Adaptor Ligation Mix Add reagents in the order listed	PN	1Χ (μl)	4X + 10% (μl)	8X + 10% (µl)
 Ligation Buffer 	2000092	20	88	176
ONA Ligase	220110/ 220131	10	44	88
Adaptor Oligos	2000094	20	88	176
Total	-	50	220	440

- **b.** Add **50 \mul** Adaptor Ligation Mix to **50 \mul** sample. Pipette mix 15x (pipette set to 90 μ l). Centrifuge briefly.
- c. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
30°C	100 μl	15 min
Step	Temperature	Time
1	20°C	00:15:00
2	4°C	Hold

3.4 Post Ligation Cleanup – SPRIselect

- a. Vortex to resuspend SPRIselect Reagent. Add 80 μ l SPRIselect Reagent (0.8X) to each sample. Pipette mix 15x (pipette set to 150 μ l).
- b. Incubate 5 min at room temperature.
- c. Place on the magnet•High until the solution clears.
- d. Remove the supernatant.
- e. Add 200 µl 80% ethanol to the pellet. Wait 30 sec.
- f. Remove the ethanol.
- g. Repeat steps e and f for a total of 2 washes.
- h. Centrifuge briefly. Place on the magnet•Low.
- i. Remove any remaining ethanol. Air dry for 2 min.
 DO NOT exceed 2 min as this will decrease elution efficiency.
- j. Remove from the magnet. Add 30.5 μ l Buffer EB. Pipette mix 15x (pipette set to 25 μ l).
- k. Incubate 2 min at room temperature.
- I. Place on the magnet•Low until the solution clears.
- m. Transfer 30 μl sample to a new tube strip.

INDE>

3.5 Sample Index PCR



- a. Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run. Record the 10x Sample Index name (PN-3000431 Dual Index Plate TT Set A well ID) used.
- b. Add 50 µl Amp Mix (PN-2000047 or 2000103) to 30 µl sample.
- c. Add 20 µl of an individual Dual Index TT Set A to each sample and record the well ID used. Pipette mix 5x (pipette set to 90 µl). Centrifuge briefly.
- d. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~25-40 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	54°C	00:00:30
4	72°C 00:00:20	
5	Go to step 2, see bel	low for # of cycles
6	72°C	00:01:00
7	4°C	Hold



The total cycles should be optimized based on 25% carry forward cDNA yield/input calculated during cDNA QC & Quantification (step 2.4)

cDNA Input	Total Cycles
0.25-25 ng	14-16
25-150 ng	12-14
150-500 ng	10-12
500-1,000 ng	8-10
1,000-1,500 ng	6-8
>1500 ng	5



e. Store at 4°C for up to 72 h or proceed to the next step.

3.6 Post Sample Index PCR Double Sided Size Selection – SPRIselect


- a. Vortex to resuspend the SPRIselect reagent. Add 60 µl SPRIselect Reagent (0.6X) to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate 5 min at room temperature.
- c. Place the magnet High until the solution clears. DO NOT discard supernatant.
- d. Transfer 150 µl supernatant to a new tube strip.
- e. Vortex to resuspend the SPRIselect reagent. Add **20 µl** SPRIselect Reagent **(0.8X)** to each sample. Pipette mix 15x (pipette set to 150 µl).
- f. Incubate 5 min at room temperature.
- g. Place the magnet•High until the solution clears.
- h. Remove $165 \,\mu l$ supernatant. DO NOT discard any beads.
- i. With the tube still in the magnet, add $200 \mu l$ 80% ethanol to the pellet. Wait 30 sec.
- i. Remove the ethanol.
- k. Repeat steps i and j for a total of 2 washes.
- l. Centrifuge briefly. Place on the magnet•Low. Remove remaining ethanol.
- m. Remove from the magnet. Add 35.5 μl Buffer EB. Pipette mix 15x (pipette set to 30 μl).
- n. Incubate 2 min at room temperature.
- o. Place on the magnet. Low until the solution clears.
- **p.** Transfer $35 \mu l$ to a new tube strip.



q. Store at 4°C for up to 72 h or at -20°C for long-term storage.

3.7
Post Library
Construction QC

Run 1 µl sample at 1:10 dilution on an Agilent Bioanalyzer High Sensitivity chip.

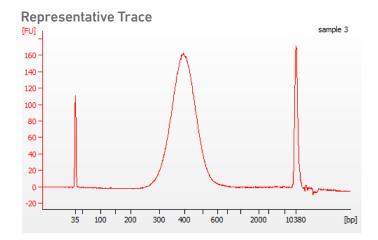

Determine the average fragment size from the Bioanalyzer trace. This will be used as the insert size for library quantification.

Alternate QC Method:

- Agilent TapeStation
- LabChip
- Fragment Analyzer

See Appendix for representative traces

See Appendix for Post Library Construction Quantification

Step 4

CRISPR Screening Library Construction

- **4.1** Guide RNA cDNA Cleanup— SPRIselect
- **4.2** Feature PCR
- **4.3** Post Feature PCR Cleanup SPRIselect
- **4.4** Sample Index PCR
- 4.5 Post Sample Index PCR Double Sided Size Selection SPRIselect
- **4.6** Post Library Construction QC

CRISPR Screening Library Construction



GET STARTE	ED!			
Action	Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room Temperature	Feature SI Primers 3 Verify name & PN Use indicated primer only	2000263	-	-20°C
DUAL INDEX		3000483	-	-20°C
	Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
	Agilent TapeStation Screen Tape and Reagents If used for QC		Manufacturer's recommendations.	-
	Agilent Bioanalyzer High Sensitivity kit If used for QC	-	Manufacturer's recommendations.	-
	DNA High Sensitivity Reagent Kit If LabChip used for QC	-	Manufacturer's recommendations.	-
Place on Ice	○ Amp Mix	2000047	Centrifuge briefly.	-20°C
	KAPA Library Quantification Kit for Illumina Platforms	-	Manufacturer's recommendations.	-
Obtain	Qiagen Buffer EB	-	-	Ambient
	10x Magnetic Separator	230003	See Tips & Best Practices.	Ambient
	Prepare 80% Ethanol Prepare 20 ml for 8 reactions	-	Prepare fresh.	Ambient

4.1 Guide RNA cDNA Cleanup – SPRIselect

- a. Vortex to resuspend the SPRIselect reagent. Add 40 μ l SPRIselect reagent (1.0X) to 40 μ l Transfered Supernatant Cleanup from step 2.3C and pipette mix 15x (pipette set to 60 μ l).
- b. Incubate 5 min at room temperature.
- c. Place on the magnet•High until the solution clears.
- **d.** Remove supernatant.
- e. Add 200 µl 80% ethanol to the supernatant. Wait 30 sec.
- f. Remove the ethanol.
- **g.** Repeat steps e and f for a total of 2 washes.
- h. Centrifuge briefly and place on the magnet•Low.



- i. Remove any remaining ethanol. Air dry for 2 min. DO NOT exceed 2 min as this will decrease elution efficiency.
- j. Remove from the magnet. Add 50.5 µl Buffer EB. Pipette mix 15x.
- k. Incubate 2 min at room temperature.
- l. Place the tube strip on the magnet•High until the solution clears.
- m. Transfer $50 \mu l$ sample to a new tube strip.



n. Store at 4°C for up to 72 h or at -20°C for up to a week, or proceed to the next step.

4.2 Feature PCR

a. Prepare Feature PCR Mix on ice. Vortex and centrifuge briefly.

Feature PCR Mix Add reagents in the order listed	PN	1Χ (μl)	4X + 10% (μl)	8X + 10% (µl)
○ Amp Mix	2000047	50	220	440
Feature SI Primers 3	2000263	45	198	396
Total	-	95	418	836



- b. Transfer ONLY 5 μl from Guide RNA cDNA Cleanup (step 4.1m) to a new tube strip. Note that only 5 μl of the DNA sample transfer is sufficient for generating CRISPR Screening library. The remaining 45 μl sample can be stored at 4°C for up to 72 h or at -20°C for up to 4 weeks, for generating additional CRISPR Screening libraries.
- c. Add 95 µl Feature PCR Mix to 5 µl sample.
- d. Pipette mix 15x (pipette set to 90 µl). Centrifuge briefly.



e. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~20 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	58°C	00:00:05
4	72°C	00:00:05
5	Go to Step 2, repeat	10X for a total of 11 cycles
6	72°C	00:01:00
7	4°C	Hold

4.3 Post Feature PCR Cleanup – SPRIselect

- a. Vortex to resuspend SPRIselect Reagent. Add 100 μ l SPRIselect Reagent (1.0X) to each sample. Pipette mix 15x (pipette set to 150 μ l).
- b. Incubate 5 min at room temperature.
- c. Place on the magnet•High until the solution clears.
- d. Remove the supernatant.
- e. Add 300 µl 80% ethanol to the pellet. Wait 30 sec.
- f. Remove the ethanol.
- g. Add 200 μ l 80% ethanol to the pellet. Wait 30 sec.
- h. Remove the ethanol.
- i. Centrifuge briefly. Place on the magnet•Low.
- j. Remove any remaining ethanol. Air dry for 2 min.
 DO NOT exceed 2 min as this will decrease elution efficiency.
- k. Remove from the magnet. Add 30.5 µl Buffer EB. Pipette mix 15x.
- I. Incubate 2 min at room temperature.
- m. Place on the magnet•Low until the solution clears.
- n. Transfer $30 \mu l$ sample to a new tube strip.

4.4 Sample Index PCR



- a. Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run. Record the 10x sample index name (PN-3000483 Dual Index Plate NT Set A well ID) used.
- b. Prepare Sample Index PCR Mix.

Sample Index PCR Mix Add reagents in the order listed	PN	1Χ (μl)	4Χ + 10% (μl)	8X + 10% (µl)
○ AmpMix	2000047	50	220	440
Buffer EB	-	25	110	220
Total	-	75	330	660

- c. Transfer ONLY 5 μ l Post Feature PCR Cleanup sample (step 4.3m) to a new tube strip. Note that only 5 μ l sample transfer is sufficient for generating CRISPR Screening library. The remaining 25 μ l sample can be stored at 4°C for up to 72 h or at –20°C for up to 4 weeks, for generating additional CRISPR Screening libraries.
- d. Add 75 μl Sample Index PCR Mix to 5 μl sample (Post Feature PCR Cleanup).
- e. Add 20 μ l of an individual Dual Index Plate NT Set A to each well and record the well ID used. Pipette mix 5x (pipette set to 90 μ l). Centrifuge briefly.



f. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~25 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	54°C	00:00:30
4	72°C	00:00:20
5	Go to step 2, repeat 8X for a total of 9 cycles	
6	72°C	00:01:00
7	4°C	Hold

4.5 Post Sample Index PCR Double Sided Size Selection – SPRIselect

- a. Vortex to resuspend the SPRIselect reagent. Add **80 µl** SPRIselect Reagent **(0.8X)** to each sample. Pipette mix 15x (pipette set to 150 µl).
- b. Incubate 5 min at room temperature.
- c. Place the magnet High until the solution clears. DO NOT discard supernatant.
- d. Transfer 170 µl supernatant to a new tube strip.
- e. Vortex to resuspend the SPRIselect reagent. Add **20 µl** SPRIselect Reagent **(1.0X)** to each sample. Pipette mix 15x (pipette set to 150 µl).
- f. Incubate 5 min at room temperature.
- g. Place the magnet•High until the solution clears.
- h. Remove the supernatant.
- i. Add 300 µl 80% ethanol to the pellet. Wait 30 sec.
- i. Remove the ethanol.
- k. Add 200 μl 80% ethanol to the pellet. Wait 30 sec.
- I. Remove the ethanol.
- m. Centrifuge briefly. Place on the magnet Low.
- n. Remove remaining ethanol. Air dry for 1 min.
- o. Remove from the magnet. Add 30.5 µl Buffer EB. Pipette mix 15x.
- p. Incubate 2 min at room temperature.
- q. Place on the magnet•Low until the solution clears.
- r. Transfer 30 μ l to a new tube strip.




s. Store at 4°C for up to 72 h or at -20°C for long-term storage.

4.6
Post Library
Construction QC

Run 1 µl sample at 1:50 dilution on an Agilent Bioanalyzer High Sensitivity chip.

Representative Trace

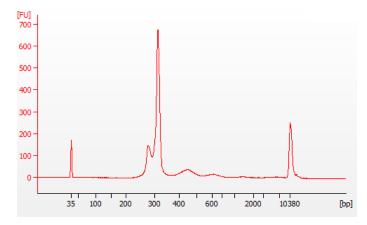

Determine the average fragment size from the Bioanalyzer trace. This will be used as the insert size for library quantification.

Alternate QC Method:

- Agilent TapeStation
- LabChip
- Fragment Analyzer

See Appendix for representative trace

See Appendix for Post Library Construction Quantification

Step 5

Cell Multiplexing Library Construction

- **5.1** Sample Index PCR
- **5.2** Post Sample Index PCR Size Selection SPRIselect
- **5.3** Post Library Construction QC



5.0 Cell Multiplexing Library Construction



GET STAR	ΓED!				
Action		Item	10x PN	Preparation & Handling	Storage
Equilibrate to Room INDEX		Dual Index Plate NN Set A Verify name & PN Use indicated plate only	3000482	-	−20°C
		Beckman Coulter SPRIselect Reagent	-	Manufacturer's recommendations.	-
		Agilent TapeStation Screen Tape and Reagents If used for QC	-	Manufacturer's recommendations.	-
		Agilent Bioanalyzer High Sensitivity kit If used for QC	-	Manufacturer's recommendations.	-
		DNA High Sensitivity Reagent Kit If LabChip used for QC	-	Manufacturer's recommendations.	-
Place on Ice	\bigcirc	Amp Mix	2000047	Centrifuge briefly.	-20°C
		KAPA Library Quantification Kit for Illumina Platforms	-	Manufacturer's recommendations.	-
Obtain	G	liagen Buffer EB	-	-	Ambient
	1	0x Magnetic Separator	230003	See Tips & Best Practices.	Ambient
	P	Prepare 80% Ethanol Prepare 20 ml for 8 eactions	-	Prepare fresh.	Ambient

INDE)

5.1 Sample Index PCR



- a. Choose the appropriate sample index sets to ensure that no sample indices overlap in a multiplexed sequencing run. Record the 10x sample index name (PN-3000482 Dual Index Plate NN Set A well ID) used.
- b. Prepare Sample Index PCR Mix.

	Sample Index PCR Mix Add reagents in the order listed	PN	1Χ (μl)	4Χ + 10% (μl)	8X + 10% (μl)
\bigcirc	Amp Mix	2000047	50	220	440
	Buffer EB	-	25	110	220
	Total	-	75	330	660

c. Transfer ONLY 5 μ l DNA sample from the Transferred Supernatant Cleanup from step 2.3B to a new tube strip.

Note that only $5 \mu l$ DNA sample is sufficient for generating Cell Multiplexing library. The remaining $35 \mu l$ DNA sample can be stored at $4^{\circ}C$ for up to 72 h or at $-20^{\circ}C$ for up to 4 weeks for generating additional Cell Multiplexing libraries.

- d. Add 75 µl Sample Index PCR Mix to each sample.
- e. Add 20 μ l of an individual Dual Index NN Set A to each sample and record the well ID used. Pipette mix 5x (pipette set to 90 μ l). Centrifuge briefly.
- f. Incubate in a thermal cycler with the following protocol.

Lid Temperature	Reaction Volume	Run Time
105°C	100 μl	~10-15 min
Step	Temperature	Time
1	98°C	00:00:45
2	98°C	00:00:20
3	54°C	00:00:30
4	72°C	00:00:20
5	Go to step 2, repeat 5X	for a total of 6 cycles
6	72°C	00:01:00
7	4°C Hold	

5.2 Post Sample Index PCR Size Selection – SPRIselect

- a. Vortex to resuspend the SPRIselect reagent. Add 120 μ l SPRIselect Reagent (1.2X) to each sample. Pipette mix 15x (pipette set to 150 μ l).
- b. Incubate 5 min at room temperature.
- c. Place on the magnet•High until the solution clears.
- d. Remove the supernatant.
- e. Add 300 µl 80% ethanol to the pellet. Wait 30 sec.
- f. Remove the ethanol.
- g. Add 200 μ l 80% ethanol to the pellet. Wait 30 sec.
- h. Remove the ethanol.
- i. Centrifuge briefly. Place on the magnet•Low. Remove remaining ethanol. Air dry for 2 min.
- j. Remove from the magnet. Add 40.5 µl Buffer EB. Pipette mix 15x.
- k. Incubate 2 min at room temperature.
- I. Place on the magnet•Low until the solution clears.
- m. Transfer $40 \mu l$ to a new tube strip.




n. Store at 4°C for up to 72 h or at -20°C for long-term storage.

5.3 Post Library Construction QC

Run 1 µl sample at 1:20 dilution on an Agilent Bioanalyzer High Sensitivity chip.



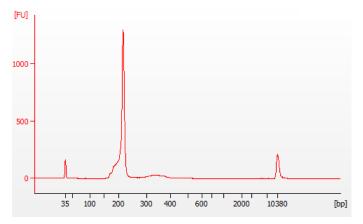

Determine the average fragment size from the Bioanalyzer trace. This will be used as the insert size for library quantification.

Alternate QC Method:

- Agilent TapeStation
- LabChip
- Fragment Analyzer

See Appendix for representative traces

See Appendix for Post Library Construction Quantification

Sequencing


Step 6 Sequencing

Sequencing Libraries

Chromium Single Cell 3' Gene Expression, CRISPR Screening, and Cell Multiplexing Dual Index libraries comprise standard Illumina paired-end constructs which begin with P5 and end with P7. These libraries include 16 bp 10x Barcodes at the start of TruSeq Read 1 and Nextera Read 1 (Read 1N) respectively while i7 and i5 sample index sequences are incorporated as the sample index read. TruSeq Read 1 and TruSeq Read 2 are standard Illumina sequencing primer sites used in paired-end sequencing of Single Cell 3' Gene Expression libraries. Nextera Read 1 (Read 1N) and TruSeq Read 2 are used in paired-end sequencing of CRISPR Screening libraries. Nextera Read 1 (Read 1N) and Nextera Read 2 (Read 2N) are used for paired-end sequencing of Cell Multiplexing libraries. Sequencing these libraries produces a standard Illumina BCL data output folder.



*Minimum required Read 2 length for Cell Multiplexing libraries is 15 bp

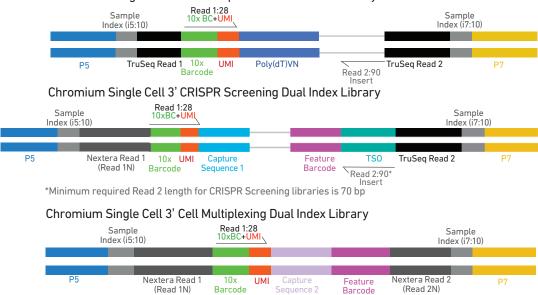

The compatibility of the listed sequencers has been verified by 10x Genomics. Some variation in assay performance is expected based on sequencer choice. For more information about performance variation, visit the 10x Genomics Support website.

Read 2:90*

- MiSeq
- NextSeq 500/550
- HiSeg 2500 (Rapid Run)
- HiSeq 3000/4000
- NovaSeq

Sample Indices

Illumina Sequencer

Compatibility

Each sample index in the Dual Index Kit TT Set A (PN-1000215), Dual Index Kit NT Set A (PN-1000242), or Dual Index Kit NN Set A (PN-1000243), is a mix of one unique i7 and one unique i5 sample index. If multiple samples are pooled in a sequencing lane, the sample index name (i.e. the Dual Index TT Set A plate well ID, SI-TT-__) is needed in the sample sheet used for generating FASTQs with "cellranger mkfastq". Samples utilizing the same sample index should not be pooled together or run on the same flow cell lane, as this would not enable correct sample demultiplexing.

Step 6 Sequencing

3' Gene Expression Library Sequencing Depth & Run Parameters

Sequencing Depth	Minimum 20,000 read pairs per cell		
Sequencing Type	Paired-end, dual indexing		
Sequencing Read	Recommended Number of Cycles		
Read 1 i7 Index i5 Index Read 2	28 cycles 10 cycles 10 cycles 90 cycles		
Sequencing Depth	Minimum 5,000 read pairs per cell		
Sequencing Type	Paired-end, dual indexing		
Sequencing Read	Recommended Number of Cycles		
Read 1 i7 Index i5 Index Read 2	28 cycles Minimum required Read 2 length for CRISPR 10 cycles Screening libraries is 70 bp 10 cycles Minimum required Read 2 length for Cell 90 cycles Multiplexing libraries is 15 bp		

CRISPR Screening and Cell Multiplexing Library Sequencing Depth & Run Parameters†

†Pooling Single Cell 3' Gene Expression, CRISPR Screening, and Cell Multiplexing dual index libraries is recommended for sequencing to maintain nucleotide diversity.

Library Loading

Once quantified and normalized, the 3' Gene Expression, CRISPR Screening, and Cell Multiplexing libraries should be denatured and diluted as recommended for Illumina sequencing platforms. Refer to Illumina documentation for denaturing and diluting libraries. Refer to the 10x Genomics Support website, for more information.

Instrument	3' Gene Expression libraries alone 3' Gene Expression + CRISPR/Cell Multiplexing libraries		
	Loading Concentration (pM)	PhiX (%)	
MiSeq	11	1	
NextSeq 500/550	1.8	1	
HiSeq 2500 (RR)	11	1	
HiSeq 4000	240	1	
NovaSeq	150*/300	1	

 $^{^{\}ast}$ Use 150pM loading concentration for Illumina XP workflow.

Library Pooling

The 3' Gene Expression, CRISPR Screening, and Cell Multiplexing libraries may be pooled for sequencing, taking into account the differences in cell number and per-cell read depth requirements between each library. Samples utilizing the same sample index should not be pooled together, or run on the same flow cell lane, as this would not enable correct sample demultiplexing.

Library Pooling Example:

Libraries	Sequencing Depth (read pairs per cell)	Library Pooling Ratio
3' Gene Expression library	20,000	4
CRISPR Screening	5,000	1
Cell Multiplexing library	5,000	1

Step 6 Sequencing

Data Analysis and Visualization

Sequencing data may be analyzed using Cell Ranger or 10x Genomics Cloud Analysis and visualized using Loupe Browser. Key features for these tools are listed below. For detailed productspecific information, visit the 10x Genomics Support website.

Cell Ranger

Cell Ranger is a set of analysis pipelines that processes Chromium Single Gene Expression data to align reads, generate Feature Barcode matrices and perform clustering and gene expression analysis.




- · Input: Base call (BCL) and FASTQ
- Output: BAM, MEX, CSV, HDF5, Web Summary, .cloupe/.loupe
- Operating System: Linux

Cloud Analysis

Cloud Analysis is currently only available for US customers.

Cloud Analysis allows users to run Cell Ranger analysis pipelines from a web browser while computation is handled in the cloud.



Input: FASTQ

• Output: BAM, MEX, CSV, HDF5, Web Summary, .cloupe/.loupe.

Loupe Browser

Loupe Browser is an interactive data visualization tool that requires no prior programming knowledge.



- Output: Data visualization, including t-SNE and UMAP projections, custom clusters, differentially expressed genes
- · Operating System: MacOS, Windows



Troubleshooting **



GEMs

STEP

NORMAL

REAGENT CLOGS & WETTING FAILURES

1.4 d After Chip G is removed from the Controller and the wells are exposed




All 8 recovery wells are similar in volume and opacity.



Recovery well G indicates a reagent clog. Recovery well C and E indicate a wetting failure. Recovery wells B, D, and F are normal. Wells A and H contain 50% Glycerol Solution.

1.4 f Transfer GEMs from Chip G Row Labeled 3



All liquid levels are similar in volume and opacity without air trapped in the pipette tips.



Pipette tips C and E indicate a wetting failure. Pipette tip C contains partially emulsified GEMs. Emulsion is absent in pipette tip E. Pipette tip G indicates a reagent clog.

STEP


NORMAL

REAGENT CLOGS & WETTING FAILURES

2.1 a After transfer of the GEMs + Recovery Agent




All liquid levels are similar in the aqueous sample volume (clear) and Recovery Agent/Partitioning Oil (pink).




Tube G indicates a reagent clog has occurred. There is a decreased volume of aqueous layer (clear).

Tube C and E indicate a wetting failure has occurred. There is an abnormal volume of Recovery Agent/Partitioning Oil (pink).

2.1 b
After aspiration of
Recovery Agent/
Partitioning Oil




All liquid volumes are similar in the aqueous sample volume (clear) and residual Recovery Agent/Partitioning Oil (pink).




Tube G indicates a reagent clog has occurred. There is a decreased volume of aqueous layer (clear). There is also a greater residual volume of Recovery Agent/Partitioning Oil (pink).

Tube C and E indicate a wetting failure has occurred. There is an abnormal residual volume of Recovery Agent/Partitioning Oil (pink).

2.1 d After addition of Dynabeads Cleanup Mix



All liquid volumes are similar after addition of the Dynabeads Cleanup Mix.



Tube 6 indicates a reagent clog has occurred. There is an abnormal ratio of Dynabeads Cleanup Mix (brown) to Recovery Agent/Partitioning Oil (appears white).

Tube C and E indicate a wetting failure has occurred. There is an abnormal ratio of Dynabeads Cleanup Mix (brown) to Recovery Agent/Partitioning Oil (appears white).

If a channel clogs or wetting failure occurs during GEM generation, it is recommended that the sample be remade. If any of the listed issues occur, take a picture and send it to support@10xgenomics.com for further assistance.

Chromium Controller Errors

- If the Chromium Controller or the Chromium Single Cell Controller fails to start, an error tone will sound and one of the following error messages will be displayed:
- a. Chip not read Try again: Eject the tray, remove and/or reposition the Chromium Next GEM Secondary Holder assembly and try again. If the error message is still received after trying this more than twice, contact support@10xgenomics.com for further assistance.
- b. Check gasket: Eject the tray by pressing the eject button to check that the 10x Gasket is correctly installed on the Chromium Next GEM Chip. If the error message persists, contact support@10xgenomics.com for further assistance.
- c. Error Detected: Row _ Pressure:
 - i. If this message is received within a few seconds of starting a run, eject the tray by pressing the eject button and check for dirt or deposits on the 10x Gasket. If dirt is observed, replace with a new 10x Gasket and try again. If the error message is still received after trying this more than twice, contact support@10xgenomics.com for further assistance.
 - ii. If this message is received after a few minutes into the run, the Chromium Next GEM Chip must be discarded. **Do not try running this Chromium Next GEM Chip** again as this may damage the Chromium Controller.
- d. Invalid Chip CRC Value: This indicates that a Chromium Next GEM Chip has been used with an older firmware version. The chip must be discarded. Contact support@10xgenomics.com for further assistance.
- **e.** Chip Holder Not Present: Open the controller drawer and check if chip holder is present. Insert chip properly into chip holder and retry.
- f. Unauthorized Chip: This indicates that an incompatible non-Next GEM chip has been used with an instrument that only can run Next GEM assays. Use only Chromium Controller (PN-120223;120246) or Chromium Single Cell Controller (PN-120263;120212) to run that chip or chip must be discarded. Contact support@10xgenomics.com for further assistance.
- **g. Endpoint Reached Early:** If this message is received, contact support@10xgenomics.com for further assistance.

Appendix

Post Library Construction Quantification Agilent TapeStation Traces LabChip Traces Oligonucleotide Sequences



Post Library Construction Quantification

- a. Thaw KAPA Library Quantification Kit for Illumina Platforms.
- **b.** Dilute $2 \mu l$ sample with deionized water to appropriate dilutions that fall within the linear detection range of the KAPA Library Quantification Kit for Illumina Platforms. (For more accurate quantification, make the dilution(s) in duplicate).
- c. Make enough Quantification Master Mix for the DNA dilutions per sample and the DNA Standards (plus 10% excess) using the guidance for 1 reaction volume below.

Quantification Master Mix	1X (μl)
SYBR Fast Master Mix + Primer	12
Water	4
Total	16

- d. Dispense 16 μ l Quantification Master Mix for sample dilutions and DNA Standards into a 96 well PCR plate.
- e. Add $4 \mu l$ sample dilutions and $4 \mu l$ DNA Standards to appropriate wells. Centrifuge briefly.
- f. Incubate in a thermal cycler with the following protocol.

Step	Temperature	Run Time	
1	95°C	00:03:00	
2	95°C	00:00:05	
3	67°C	00:00:30	
	Read signal		
4	Go to Step 2, 29X (Total 30 cycles)		


g. Follow the manufacturer's recommendations for qPCR-based quantification. For library quantification for sequencer clustering, determine the concentration based on insert size derived from the Bioanalyzer/TapeStation trace.

Agilent TapeStation Traces

Agilent TapeStation Traces


Agilent TapeStation High Sensitivity D5000 ScreenTape was used.Protocol steps correspond to the Chromium Next GEM Single Cell 3' (Dual Index) v3.1 User Guide with Feature Barcode technology for CRISPR Screening and Cell Multiplexing (CG000389)

Protocol Step 2.4 - cDNA QC & Quantification

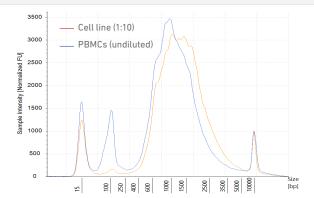


Run 2 μ l sample mixed with 2 μ l loading buffer. Ensure dilution factor is factored in when calculating cDNA yield/ μ l (divide by 2).

Protocol Step 3.7 - Post Library Construction QC



Run 2 μ l diluted sample (1:10 dilution) mixed with 2 μ l loading buffer.

Protocol Step 4.6 – Post Library Construction QC (CRISPR Screening library)



Run 2 μ l diluted sample (1:50 dilution) mixed with 2 μ l loading buffer.


All traces are representative.

Agilent TapeStation Traces

Agilent TapeStation Traces

Agilent TapeStation High Sensitivity D5000 ScreenTape was used.Protocol steps correspond to the Chromium Next GEM Single Cell 3' (Dual Index) v3.1 User Guide with Feature Barcode technology for CRISPR Screening and Cell Multiplexing (CG000389)

Protocol Step 5.3 – Post Library Construction QC (Cell Multiplexing library)



Run 2 μ l diluted sample (1:20 dilution) mixed with 2 µl loading buffer.

All traces are representative.

LabChip Traces


LabChip Traces

DNA High Sensitivity Reagent Kit was used.


Protocol steps correspond to the Chromium Next GEM Single Cell 3' v3.1 (Dual Index) User Guide with Feature Barcode technology for CRISPR Screening and Cell Multiplexing (CG000389)

Protocol Step 2.4 - cDNA QC & Quantification

Run 10 µl sample. cDNA yield calculation is same as Agilent Bioanalyzer traces.

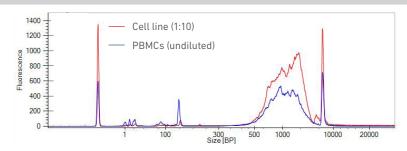


Protocol Step 3.7 - Post Library Construction QC

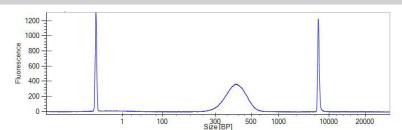


Run 10 µl diluted sample (1:10 dilution).

Protocol Step 4.6 – Post Library Construction QC (CRISPR Screening Library)

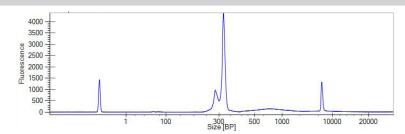

Run 10 µl diluted sample (1:50 dilution).

Protocol Step 5.3 – Post Library Construction QC (Cell Multiplexing library)

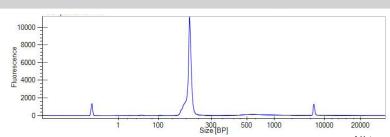

Run 10 µl diluted sample (1:20 dilution).

All traces are representative.

Alternate QC Method:

Qubit Fluorometer and Qubit dsDNA HS Assay Kit

Multiply the cDNA concentration reported via the Qubit Fluorometer by the elution volume (40 μ l) to obtain the total cDNA yield in ng. To determine the equivalent range using the Agilent 2100 Expert Software, select the region encompassing 35–10,000 bp.

Compatible sgRNA Specifications


Integration of Capture Sequence 1 and Capture Sequence 2 in sgRNA

A representative sgRNA sequence along with the specific capture sequences integrated in two different locations in the sgRNA are shown


Capture Sequence 1

Capture Sequence 1 on Gel Bead: 5'-TTGCTAGGACCGGCCTTAAAGC-3'

Capture Sequence 1 integrated in sgRNA hairpin




Capture Sequence 1 integrated in sgRNA 3'-end



Capture Sequence 2


Capture Sequence 2 on Gel Bead: 5'-CCTTAGCCGCTAATAGGTGAGC-3'

Capture Sequence 2 integrated in sgRNA hairpin



5-NNNNNNNNNNNNNNNNNNNTTTAAGAGCTAAGCTGGAAACAGCATAGCAAGTTTAAATAAGGCTAGTCCGTTATCAACTTggccGCTCACCTATTAGCGGCCTAAGCGGgccAAGTGGCACCGAGTCCGTTCTTTTT-3

Capture Sequence 2 integrated in sgRNA 3'-end



5-NNNNNNNNNNNNNNNNNNNTTTAAGAGCTAAGCTGGAAACAGCATAGCAAGTTTAAATAAGGCTAGTCCGTTATCAACTTgaaaAAGTGGCACCGAGTCGGTCCCCTCACCTATTAGCGGCTCAAGCTTTTTTT-3


Oligonucleotide Sequences


Protocol steps correspond to the Chromium Next GEM Single Cell 3' (Dual Index) v3.1 User Guide with Feature Barcode technology for Cell Multiplexing (CG000xxx) Protocol Step 1.5 - GEM-RT Incubation Gel Bead Primers TruSeq Read 1 Barcode Poly(dT)VN Capture Sequence Gel Bead Capture Sequence 2 5'-GTCAGATGTGTATAAGAGACAG-N16-N12-TTGCTAGGACCGGCCTTAAAGC-3' 5'-GTCAGATGTGTATAAGAGACAG-N16-N12-CCTTAGCCGCTAATAGGTGAGC-3' Template Switch Oligo PN-3000228 5'-AAGCAGTGGTATCAACGCAGAGTACATrGrGrG-3' Lipid Cell Multiplexing Capture Seq 2 Feature Barcode Read 2N Molecule Oligo Feature Barcode 3'-GGAATCGGCGATTATCCACTCG-N15-GACAGAGAATATGTGTAGAGGCTCGGGTGCTCTG-5' cDNA from poly-adenylated mRNA GEM-RT **Products** TS0 10x Barcode UMI Poly(dT)VN cDNA from sgRNA Partial Read 1N 10x Barcode UMI Capture Sequence 1 Feature Barcode TS0 (sgRNA Protocospacer) 5'-GTCAGATGTGTATAAGAGACAG-N16-N12-TTGCTAGGACCGGCCTTAAAGC-sgRNA_Feature_Barcode-CCCATGTACTCTGCGTTGATACCACTGCTT-3' DNA from Cell Multiplexing Oligo Feature Barcode Read 2N Read 1N 10x Barcode UMI Capture Seq 2 Feature Barcode 5'-GTCAGATGTGTATAAGAGACAG-N16-N12-CCTTAGCCGCTAATAGGTGAGC-N15-CAGAGCACCCGAGCCTCTACACATATTCTCTGTC-3'

Oligonucleotide Sequences

Protocol steps correspond to the Chromium Next GEM Single Cell 3' (Dual Index) v3.1 User Guide with Feature Barcode technology for Cell Multiplexing (CG000xxx) Protocol Step 2.2 - cDNA Amplification Feature cDNA **Amplifies cDNA** Primers 3 PN-2000289 Forward Primer: Reverse Primer: Partial Read 1 5'-CTACACGACGCTCTTCCGATCT-3' 5'-AAGCAGTGGTATCAACGCAGAG-3' Amplifies cDNA from sgRNA Forward Primer: Reverse primer: Partial TSO 5'-GCAGCGTCAGATGTGTATAAGAGACAG-3' 5'-AAGCAGTGGTATCAACGCAGAG-3' Amplifies DNA from Cell Multiplexing Oligo Feature Barcode Forward Primer: Reverse primer: Partial Read 2N 5'-GCAGCGTCAGATGTGTATAAGAGACAG-3' 5'-GTCTCGTGGGCTCGGAGATGTGTATAA-3' Amplified cDNA from poly-adenylated mRNA Amplification **Products** Read 1 10x Barcode UMI Poly(dT)VN TS₀ Amplified cDNA from sgRNA Partial Read 1N 10x Barcode UMI Feature Barcode TS₀ 5'-GCAGCGTCAGATGTGTATAAGGACAG-N16-N12-TTGCTAGGACCGGCCTTAAAGC-sgRNA_Feature_Barcode-CCCATGTACTCTGCGTTGATACCACTGCTT-3' 3'-CGTCGCAGTCTACACATATTCTCTGTC-N16-N12-AACGATCCTGGCCGGAATTTCG-sgRNA_Feature_Barcode-GGGTACATGAGACGCCAACTATGGTGACGAA-5' Amplified DNA from Cell Multiplexing Oligo Feature Barcode Read 1N 10x Barcode UMI Capture Seq 2 Feature Barcode

5'-GCAGCGTCAGATGTGTATAAGAGACAG-N16-N12-CCTTAGCCGCTAATAGGTGAGC-N15-CAGAGCACCCGAGCCTCTACACATATTCTCTGTC-3'
3'-CGTCGCAGTCTACACATATTCTCTGTC-N16-N12-GGAATCGGCGATTATCCACTCG-N15-GTCTCGTGGGCTCGGAGATGTGTATAAGAGACAG-5'

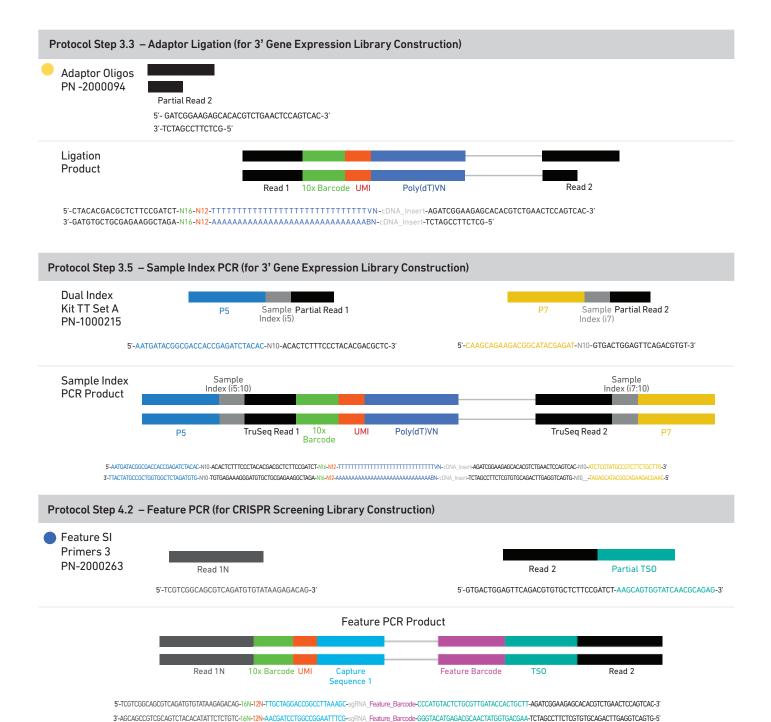

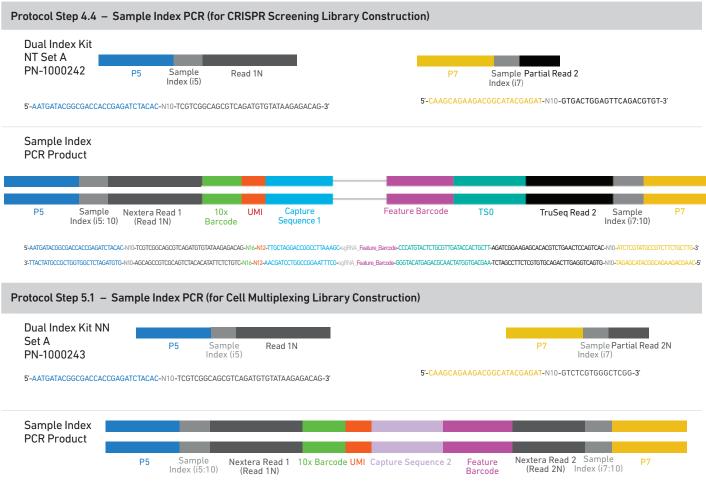

5-AATGATACGGCGACCACCGAGATCTACAC-NIO-TCGTCGGCAGCGTCAGATGTGTATAAGAGACAG-NI6-NI2-CCTTAGCCGCTAATAGGTGAGC-NI5-CAGAGCACCCGAGCCTCTACACATATTCTCTGTC-NIO-ATCTCGTATGCCGCTTCTCGCTTG-3'
3-TTACTATGCCGCTGGGCTCTAGATGTG-NIO-AGCAGCCGTCGCAGTCTACACATATTCTCTGTC-NI6-NI2-GGAATCGGCGATTATCCACTCG-NI5-GTCTCGTGGGCTCGGAGATGTGTAAAGAGACAG-NI0-TAGAGCATACCGCAGAAGACAC-5'