


10x Genomics®

Sample Preparation Demonstrated Protocol

Removal of Dead Cells from Single Cell Suspensions
for Single Cell RNA Sequencing

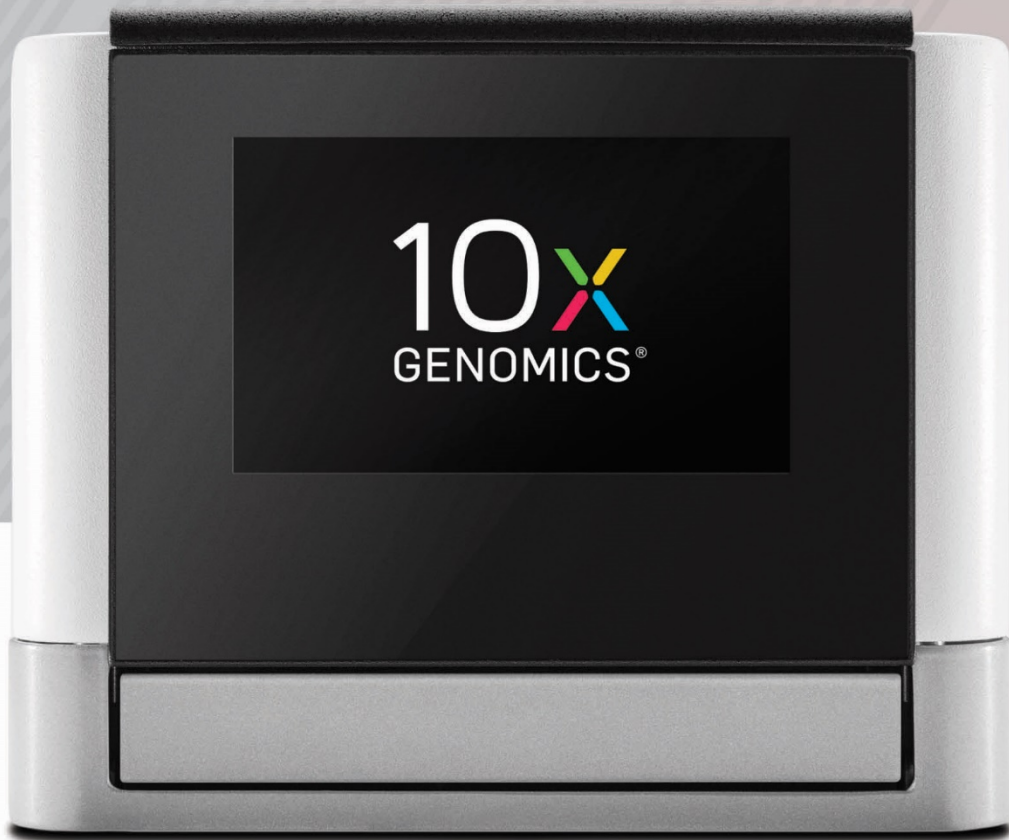

Notices

Manual Part Number

CG000093 Rev A

Legal Notices

© 2017 10x Genomics, Inc. All rights reserved. Duplication and/or reproduction of all or any portion of this document without the express written consent of 10x Genomics, Inc., is strictly forbidden. Nothing contained herein shall constitute any warranty, express or implied, as to the performance of any products described herein. Any and all warranties applicable to any products are set forth in the applicable terms and conditions of sale accompanying the purchase of such product. 10x Genomics provides no warranty and hereby disclaims any and all warranties as to the use of any third party products or protocols described herein. The use of products described herein is subject to certain restrictions as set forth in the applicable terms and conditions of sale accompanying the purchase of such product. "10x", "10x Genomics", "Changing the Definition of Sequencing", "Chromium", "GemCode", "Loupe", "Long Ranger", "Cell Ranger" and "Supernova" are trademarks of 10x Genomics, Inc. All other trademarks are the property of their respective owners. All products and services described herein are intended FOR RESEARCH USE ONLY and NOT FOR USE IN DIAGNOSTIC PROCEDURES.

The use of 10x Product(s) in practicing the methods set forth herein has not been validated by 10x, and such non-validated use is NOT COVERED BY 10X STANDARD WARRANTY, AND 10X HEREBY DISCLAIMS ANY AND ALL WARRANTIES FOR SUCH USE.

Nothing in this document should be construed as altering, waiving or amending in any manner 10x Genomics, Inc., terms and conditions of sale for the Chromium™ Controller or the Chromium Single Cell Controller, consumables or software, including without limitation such terms and conditions relating to certain use restrictions, limited license, warranty and limitation of liability, and nothing in this document shall be deemed to be Documentation, as that term is set forth in such terms and conditions of sale. Nothing in this document shall be construed as any representation by 10x Genomics, Inc that it currently or will at any time in the future offer or in any way support any application set forth herein.

Customer Information and Feedback

For technical information or advice, please contact our Customer Technical Support Division online at any time.

Email: support@10xgenomics.com

10x Genomics

7068 Koll Center Parkway

Suite 401


Pleasanton, CA 94566 USA

Table of Contents

Demonstrated Protocol	1
1. Overview	2
2. Getting Started	2
2.1. Tips & Safety	2
2.2. General Materials	3
2.3. Preparation – Buffers	4
2.4. Cell Preparation & Sourcing	4
3. Dead Cell Removal & Washing	4
4. Viability Results	5

Demonstrated Protocol

Removal of Dead Cells from
Single Cell Suspensions for
Single Cell RNA Sequencing



1. Overview

A high percentage of non-viable cells may impact the targeted cell recovery in 10x Genomics® Single Cell Protocols. This Demonstrated Protocol outlines best practices for reducing the percentage of non-viable or dead cells from a single cell suspension.

This Protocol was demonstrated using peripheral blood mononuclear cells (PBMCs) and dissociated tissue cells from colorectal cancer (CRC) and clear cell renal carcinoma (CCRC) patients. However, it may be used as a basis for removing dead cells from other cell lines as well as other primary cells in preparation for use in 10x Genomics Single Cell Protocols.

2. Getting Started

2.1. Tips & Safety

Best practices for handling any cell line includes using sterile techniques, nuclease-free reagents and consumables, minimizing pipetting steps, and using wide-bore pipette tips when possible to minimize cell damage. Transfer pipettes may be used to remove supernatant after centrifugation to minimize disturbance of the cell pellet.

To determine accurate cell counts, best practices include sampling the cell suspension at least twice and at least two counts on each sample (*i.e.* a minimum of four counts in total, based on two independent draws from the cell suspension). Consult Technical Note *Guidelines on Accurate Target Cell Counts* (Document CG000091) for more information.

CRITICAL!

Human and animal cells carry potentially hazardous pathogens. Primary tumor cells should be handled under BSL-2 conditions. Follow material supplier recommendations and local laboratory procedures and regulations for the safe handling, storage and disposal of biological materials.

2.2. General Materials

Supplier	Description	Part Number (US)
-	Refrigerated Benchtop Centrifuge for 15 ml and 50 ml tubes Microcentrifuge for 2 ml LoBind tubes Heated Water Bath, 2 l	- - -
Corning Cellgro	Phosphate-Buffered Saline (PBS) 1X without calcium & magnesium	21-040-CV
Sigma-Aldrich	Phosphate-Buffered Saline (PBS) with 10% Bovine Albumin	SRE0036
Miltenyi Biotec	MACS [®] Dead Cell Removal Kit MS Columns LS Columns MACS Multistand OctoMACS [™] Separator	130-090-101 130-042-201 130-042-401 130-042-303 130-042-109
Bel-Art	Flowmi [™] Cell Strainer, 40 µm	H13680-0040
Thermo Fisher Sci	Trypan Blue Stain (0.4%) for use with the Countess [®] Automated Cell Counter Countess II FL Automated Cell Counter Countess II Automated Cell Counting Chamber Slides Nuclease-Free Water	T10282 AMQAF1000 C10228 AM9937
Eppendorf	DNA LoBind Tubes, 2.0 ml*	022431048
Integra	PIPETBOY acu 2	155018
VWR	Sterile Polypropylene Centrifuge Tubes with Flat Caps, 50 ml Sterile Polypropylene Centrifuge Tubes with Flat Caps, 15 ml	82018-050 21008-103

*No substitutions are allowed. Items have been validated by 10x Genomics[®] and are required for Single Cell workflow, training and system operations.

2.3. Preparation – Buffers

- a) Prepare 1X PBS containing 0.04% weight/volume BSA (400 µg/ml) for the final resuspension.
- b) Prepare 1X Binding Buffer from the 20X Binding Buffer stock solution provided in the MACS® Dead Cell Removal Kit with Nuclease-Free Water.

2.4. Cell Preparation & Sourcing

- a) This Protocol assumes human PBMCs were thawed, washed and counted as described in *Demonstrated Protocol Fresh Frozen Human Peripheral Blood Mononuclear Cells* (Document CG00039).
- b) Dissociated tissue cells from CRC and CCRC patients were acquired from Conversant Bio. The cells were thawed, washed and counted per the Conversant Bio protocol, except the steps describing the DNase I treatment of the cells were omitted. Conversant Bio protocols can be found at www.conversantbio.com.

3. Dead Cell Removal & Washing

NOTE

This Protocol was demonstrated using sample sizes compatible with Miltenyi Biotec MS columns (1×10^4 – 1×10^7 labeled cells in 1×10^4 – 2×10^8 total cells). If using sample sizes compatible with Miltenyi Biotec LS columns (1×10^5 – 1×10^8 labeled cells in 1×10^7 – 2×10^9 total cells), consult the manufacturer's instructions for more information.

- a) Centrifuge the cell sample at **300 rcf** for **5 min** (PBMCs) or **10 min** (dissociated tumor cells).
- b) Remove supernatant without disturbing pellet. Add **100 µl** Dead Cell Removal MicroBeads and resuspend pelleted cells using a **wide-bore** pipette tip.
- c) Incubate for **15 min** at **room temperature** (20 – 25°C).
- d) Rinse the MS column with **500 µl** 1X Binding Buffer while the cells are incubating with the Dead Cell Removal MicroBeads.

NOTE

If using the LS column, consult the manufacturer's instructions for more information.

- e) After incubation is complete, dilute the cell suspension (containing Dead Cell Removal MicroBeads) with **500 µl** 1X Binding Buffer.
- f) Apply cell suspension to the prepared column. The positively selected dead cells will be retained on the column while the negatively selected live cells pass through the column.

CRITICAL!

Do not apply the plunger supplied with the column, otherwise positively selected dead cells will be collected in the effluent.

- g) Collect the effluent containing the live cell fraction in a sterile 15 ml polypropylene centrifuge tube.
- h) Rinse the column with **2 ml** 1X Binding Buffer and combine with the original effluent.

NOTE

If using the LS column, consult the manufacturer's instructions for more information.

DEMONSTRATED PROTOCOL Dead Cell Removal

- i) Centrifuge cells at **300 rcf** for **5 min** (PBMCs) or **10 min** (dissociated tumor cells).
- j) Remove the supernatant without disturbing the pellet.
- k) Using a **wide-bore** pipette tip, add **1 ml** 1X PBS containing 0.04% BSA to each tube and gently pipette mix 5 times to resuspend cell pellet. Transfer the cell suspension to a 2 ml tube.
- l) Centrifuge cells at **300 rcf** for **5 min** (PBMCs) or **10 min** (dissociated tumor cells).
- m) Remove the supernatant without disturbing the pellet.
- n) Repeat steps k – m for a total of two washes.
- o) Resuspend pellet in 1X PBS with 0.04 % BSA using a **wide-bore** pipette tip. Gently pipette mix 10 – 15 times or until cells are completely suspended.
- p) Determine the cell concentration using a Countess® II FL Automated Cell Counter. The target cell concentration is $\sim 7 \times 10^5$ cells/ml (700 cells/ μ l).
- q) If necessary, dilute the cells with additional 1X PBS with 0.04% BSA until the target cell concentration is reached.
- r) Once the target cell concentration is obtained, place the cells on ice.
- s) Proceed with the 10x Genomics® Single Cell Protocol.

Repeat

NOTE

The number of cells recovered in this Protocol varies depending on both the fraction of non-viable cells or dead cells present in the sample and the total concentration of cells loaded onto the column.

4. Viability Results

To demonstrate the efficiency of this Protocol, a PBMCs sample containing a high percentage of non-viable or dead cells was used. The results obtained following this Protocol are outlined below. To determine percent viability, cells were stained with trypan blue and counted using a Countess II FL Automated Cell Counter.

Sample	Sample Size Before Removal	% Live Before	% Live After
PBMCs	1.0×10^6 total cells	49%	85%
Colorectal cancer	6.5×10^6 total cells	55%	80%
Clear cell renal carcinoma	3.7×10^6 total cells	30%	70%