

HumaPen SAVVIO® INSULIN DELIVERY DEVICE INSTRUCTIONS FOR USE



INTRODUCTION

HumaPen SAVVIO® Pen is designed for ease of use. You can give yourself multiple doses from one Lilly 3 ml insulin cartridge (100 IU/ml or units/ml). You can inject from 1 to 60 units of insulin from a Lilly 3 ml insulin cartridge in each injection. You can dial your dose one (1) unit at a time. If you dial the wrong dose, you can correct the dose without wasting any insulin.

Read these instructions completely and follow the directions carefully before using the pen. Failure to follow the instructions may result in the wrong insulin dose being delivered.

DO NOT SHARE YOUR PEN OR NEEDLES AS THIS MAY RISK TRANSMISSION OF INFECTIOUS AGENTS.

If any of the parts of your Pen appear broken or damaged, DO NOT USE. Contact your local Lilly affiliate office (see end of leaflet for contact details) or your healthcare professional for a replacement Pen.

HumaPen SAVVIO is not recommended for the blind or visually impaired without the assistance of a sighted individual trained to use it.

Always carry a spare insulin pen in case your pen is lost or damaged.

IMPORTANT NOTES

- Your healthcare professional has prescribed the type of insulin best for you. Any changes in insulin should be made only under medical supervision.
- HumaPen SAVVIO is for use only with Lilly 3 ml insulin cartridges.**
- Do not use other brands of insulin cartridges.**
- Before each injection, read the cartridge label and be sure the pen contains the correct Lilly 3 ml insulin cartridge.
- The colour of the pen is not intended to indicate insulin type.

INSERT THE CARTRIDGE

- Read and follow the instructions provided in your Lilly 3 ml insulin cartridge Information for the Patient (package leaflet).
- Check to make sure the insulin cartridge is not cracked or broken and your insulin is not expired before inserting the insulin cartridge into your pen.
- Check the cartridge label for the type of insulin and appearance before each injection.

ATTACH NEEDLE

- HumaPen SAVVIO is suitable for use with BD (Becton, Dickinson and Company) Pen needles.
- Use a new needle for each injection. This will help ensure sterility. It will also help prevent leakage of insulin, keep out air bubbles, and reduce needle clogs.
- The directions regarding needle handling are not intended to replace local, healthcare professional or institutional policies.

PRIME THE PEN

- Prime every time. The pen must be primed until you see insulin at the needle tip before each injection to make sure the pen is ready to dose.
- If you do not prime, you may get the wrong dose.

INJECT THE DOSE

- HumaPen SAVVIO will not allow you to dial more than the number of units left in the cartridge.
- Do not push down on the injection button while dialling your dose.
- Do not attempt to inject your insulin by turning the dose knob. You will NOT receive your insulin by turning the dose knob. You must PUSH the injection button straight in for the dose to be delivered.
- Do not attempt to change the dose while injecting.
- You may see a drop of insulin at the needle tip. This is normal and it does not affect the dose you just received.

CARE AND STORAGE

- Remove the needle after every use. Do not store the pen with the needle attached.
- Keep your HumaPen Savvio, Lilly 3 ml insulin cartridges, and needles out of the reach and sight of children.
- Keep the pen away from moisture, dust, extreme hot or cold temperatures, and direct sunlight.
- Do not store the pen in a refrigerator.
- Wipe the pen cap, pen body and case with a damp cloth to clean them.
- Do not use alcohol, hydrogen peroxide or bleach on the pen body or dose window. Also, do not cover in liquid or apply lubrication such as oil, as this could damage the pen.
- Refer to the insulin cartridge Information for the Patient (package leaflet) for complete insulin storage instructions.

REPLACEMENT

Do not use your pen for more than 6 years after the first use or past the expiration date on the carton.

Contact your healthcare professional if a prescription is necessary, or go directly to a pharmacy when you need a new HumaPen SAVVIO.

If you have any questions or problems with your HumaPen SAVVIO Pen, contact your local Lilly affiliate office or your healthcare professional for assistance.

Record the date your Pen was first used here:

DAY _____ MONTH _____ YEAR _____

FREQUENTLY ASKED QUESTIONS

QUESTIONS ABOUT INSERTING THE CARTRIDGE

1. Why doesn't the screw move out when there is no cartridge in the pen?

The Screw may not move out when you push the injection button unless there is a cartridge in the pen. Once a cartridge is inserted, then the screw will move out when the injection button is pushed.

2. What should I do if I can't attach the cartridge holder to the pen body?

Check that the Lilly 3 ml insulin cartridge is correctly inserted into the cartridge holder. Then carefully line up the cartridge holder with the pen body and twist together until secure.

QUESTIONS ABOUT PRIMING THE PEN

1. Why is it important to prime before every injection?

- Priming helps to ensure that the pen and needle are working properly.
- Priming removes air that may collect in the needle or insulin cartridge during normal use.

If you do NOT prime, you may get the wrong insulin dose.

Priming helps to ensure that the pen and needle are working properly. Once the pen is properly primed, insulin will flow from the needle. You may need to prime several times before you see insulin at the tip of the needle.

2. Why can it take several attempts to prime when a new cartridge is inserted?

There may be a gap between the screw and the cartridge plunger. Repeating the priming steps will move the screw out to touch the cartridge plunger. Once the end of the screw pushes the cartridge plunger out, insulin will flow from the needle.

3. Why should I prime until I see insulin at the tip of the needle?

Priming moves the screw into contact with the cartridge plunger and gets the air out of the cartridge.

- You may see insulin on the tip of the needle when you first attach it. This only shows that the needle is attached and not clogged. You must still prime the pen.

- You may also see no insulin at all when you are priming pen. This may be because the screw is moving forward to close a gap between the screw and the cartridge plunger.

- Insulin will flow only when the pen is properly primed.

- If the injection button is hard to push, the needle may be clogged.

Attach a new needle. Repeat the priming steps until insulin is seen at the needle tip.

If you are still unable to see insulin flow from the needle, do NOT use the pen. Contact your healthcare professional for assistance or to obtain a replacement.

4. What should I do if I have an air bubble in the cartridge?

Priming your pen will remove air. Point the pen up, and tap the cartridge gently with your finger so any air bubbles can collect near the top. Repeat the priming steps until insulin is seen at the tip of the needle. A small air bubble may remain in the cartridge after completion of the priming steps. If you have properly primed the pen, this small air bubble will not affect your insulin dose.

QUESTIONS ABOUT INJECTING

1. What should I do if I dial a wrong dose (too high or too low)?

Turn the dose knob backward or forward to correct the dose before injecting.

2. What should I do if my full dose cannot be dialled?

If your dose is greater than the number of units left in the cartridge, you may either inject the amount remaining in your current cartridge, and then use a new cartridge to complete your dose, OR inject the full dose with a new cartridge.

For example, if you need 31 units and only 25 units remain in the cartridge you will not be able to dial past 25. In this instance you will need an additional 6 units.

Do not attempt to dial past this point. You may either:

- Inject the partial dose and then inject the remaining dose using a new cartridge.

OR

- Inject the full dose with a new cartridge.

3. Why is it difficult to push the injection button when I try to inject?

- Your needle may be clogged. Try attaching a new needle, and then prime the pen.

- Place your thumb directly on top of the injection button so the dose knob can turn freely.

- Pushing the injection button down quickly may make the button harder to push. Pushing the button more slowly may make it easier.

- Using a larger diameter needle will make it easier to push the injection button during injection. Ask your healthcare professional which needle is best for you.

If none of the above steps resolves the problem, your pen may need to be replaced.


Your Injection Button may become harder to push if the inside of your pen gets dirty with insulin, food, drink or other materials. Following the CARE AND STORAGE instructions should prevent this.

If you have any questions or problems with your HumaPen Savvio Pen, contact your local Lilly affiliate office or your healthcare professional for assistance.

MAKE SURE YOU HAVE ALL YOUR PEN COMPONENTS.

Wash your hands before each injection.

PEN NEEDLE (sold separately) HUMAPEN SAVVIO PEN PARTS

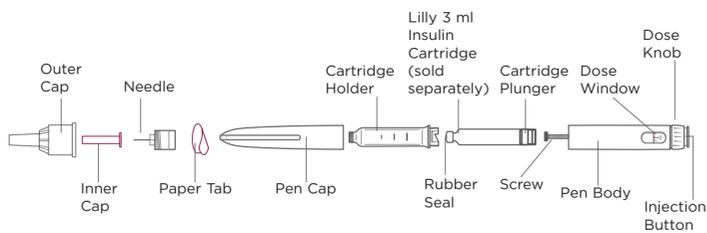

Be sure to check your insulin cartridge for:


- Type of Insulin
- Appearance
- Expiration Date
- Cracks or breakage

1. INSERT THE CARTRIDGE

Pull off pen cap and set aside.



Twist cartridge holder to detach.




Insert small end of Lilly 3 ml insulin cartridge into the cartridge holder.



If the screw is out, use the cartridge plunger to push it back.



Push the cartridge holder and pen body straight together. Twist the cartridge holder onto the pen body until **you feel a click and** it is secure.



Wipe the small rubber seal on the end of the cartridge with an alcohol swab.

FOR CLOUDY INSULIN ONLY

Follow these instructions before each injection.

Roll the pen gently 10 times.

Invert the pen gently 10 times. The insulin should look evenly mixed.



2. ATTACH NEEDLE


Remove the paper tab and discard.

Screw needle straight onto the cartridge holder until secure.



Pull off outer needle cap. Save the outer needle cap to remove the needle after your injection.

Pull off inner needle cap and throw it away.




Keep Discard

3. PRIME THE PEN BEFORE EVERY INJECTION

A new cartridge may need to be primed several times before you see insulin at the needle tip.

Dial 2 units




Point pen up. Tap cartridge to collect air at the top for removal.



Push Injection Button. Look for insulin at the tip of the needle. If no insulin is seen repeat priming.


CAUTION: If you do not prime, you may get the wrong dose.

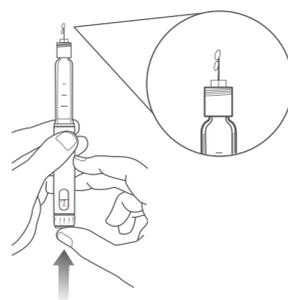

CAUTION: If no insulin is seen after several attempts, attach a new needle, as the one on your pen may be clogged.

4. INJECT THE DOSE

Turn dose knob to your desired dose. Example: 28 units is shown in the drawing below.



CAUTION: If you dial too many units, you can correct the dose by dialling backwards.

Note: The Pen will not allow you to dial more than the number of units left in the cartridge.


The dose knob clicks as you turn it. **DO NOT** dial your dose by counting clicks because you may dial the wrong dose.

Insert Needle into skin using injection technique recommended by your healthcare professional.

Place your thumb on the injection button and then **slowly** and firmly push the injection button until it stops moving.

Continue to hold the button for **5 seconds** then remove the needle from your skin.

Note: After removal check to make sure you see **0** in the dose window to confirm you received the complete dose. If you are not sure you injected your full dose, **do not inject another dose.** Call your local Lilly affiliate office or your healthcare provider.



5. STORE YOUR PEN


Carefully replace the outer needle cap as instructed by your healthcare professional.

CAUTION: To prevent air from entering the cartridge, do not store the Pen with Needle attached.




While grasping cartridge holder, unscrew the capped needle.

- Put used needles in a sharps container or a hard plastic container with a secure lid. Do not throw needles directly into your household waste.
- Do not recycle the filled sharps container.
- Ask your healthcare provider about options to dispose of the sharps container properly.
- The directions regarding needle handling are not intended to replace local, healthcare provider or institutional policies.



Replace the Pen Cap.



If you have any questions or problems with your HumaPen SAVVIO Pen, contact your local Lilly affiliate office (see below) or your healthcare professional for assistance.

Local Lilly affiliate contact details

Eli Lilly Australia Pty Limited
112 Wharf Road
West Ryde NSW 2114
Australia
Tel: 1800 023 764

Eli Lilly and Company (Ireland) Limited
Dunderrow, Kinsale
Co. Cork
Ireland
Tel: +353 (0) 1 661 4377

Eli Lilly and Company (NZ) Limited
Level 1, 123 Ormiston Rd
Botany South, Auckland
New Zealand
Tel: 0800 500 056

Eli Lilly (S.A.)(Pty) Limited
First Floor, Golden Oaks House
Ballyoaks Office Park
35 Ballyclare Drive
Bryanston
South Africa, 2191
Tel: +27 11 510 9300

Eli Lilly and Company Limited
Lilly House, Priestley Road
Basingstoke, Hampshire, RG24 9NL
United Kingdom
Tel: +44 (0) 1256 315000

Eli Lilly and Company
Pharmaceutical Delivery Systems
Lilly Corporate Center
Indianapolis, IN 46285, USA



Eli Lilly Nederland B.V.
Papendorpsweg 83,
3528 BJ UTRECHT
The Netherlands

Importer:
Lilly S.A.
Avenida. Industria 30
28108 Alcobendas,
Madrid, Spain

HumaPen SAVVIO meets the dose accuracy and functional requirements of ISO 11608-1 with Lilly 3 ml cartridges.

CE
0344

HumaPen® and HumaPen SAVVIO® are trademarks of Eli Lilly and Company.

Copyright © 2011, 2019 Eli Lilly and Company. All rights reserved.

Revision date: February 2019

Lilly

PA001SPEX04