



4141 MacArthur Blvd. • Newport Beach, CA 92660  
800-777-0695 • Fax 800-411-9722 • [glidewell dental.com](http://glidewell dental.com)

Fill out all applicable criteria on the Rx

Dr. Name \_\_\_\_\_ Phone # \_\_\_\_\_

Patient Name \_\_\_\_\_ Acct. # \_\_\_\_\_  
First Last

Address \_\_\_\_\_

Email \_\_\_\_\_ Deliver by 5 p.m. on See Reverse for Working Times

Enclosed with case: ☐ Impressions ☐ Models ☐ Bite ☐ Photos ☐ Other: \_\_\_\_\_

**FINAL BIOTEMPS SHADE**



Indicate Shade Here \_\_\_\_\_

**CHOOSE RESTORATION**

☐ **BioTemps Provisionals**

• 6-month warranty

Reinforcement:

☐ None ☐ Wire\* ☐ Fiber

☐ Cast-Metal Substructure  
+ 1 working day

☐ Cement-on Implant #(s) \_\_\_\_\_

☐ Screw-retained Implant #(s) \_\_\_\_\_

☐ **Transition Crowns & Bridges**

• Transition C&B are milled from an  
acetal resin block  
(No reinforcement)

• 2-year warranty

Fabricate:

☐ Lab Prep

☐ Solid Model

☐ Die-Trim Model

☐ Cement-on Implant #(s) \_\_\_\_\_

☐ Screw-retained Implant #(s) \_\_\_\_\_

☐ **Smile Transitions**

☐ Upper ☐ Lower  
☐ Both Arches/Quadrants

Shade \_\_\_\_\_

☐ Cosmetic Appliance

☐ Diagnostic Appliance

☐ Transitional Implant Appliance

☐ Fabricate with occlusal holes

☐ Fabricate without occlusal holes

☐ Open bite \_\_\_\_\_ mm anteriorly

☐ Add length to gingival on tooth  
#(s) \_\_\_\_\_ by \_\_\_\_\_ mm

☐ Pontic site healing, prepare  
deep ovate socket on tooth

#(s) \_\_\_\_\_ by \_\_\_\_\_ mm

**TOOTH NUMBER** #(s) \_\_\_\_\_ to \_\_\_\_\_

Abutment\* #(s) \_\_\_\_\_

Pontic #(s) \_\_\_\_\_

Extract #(s) \_\_\_\_\_

Veneer #(s) \_\_\_\_\_

Splinted\* #(s) \_\_\_\_\_

Individual units #(s) \_\_\_\_\_

Amount of Prep Reduction: ☐ 1 mm\* ☐ 2 mm

☐ Open Trench #(s) \_\_\_\_\_

**SELECT INCISAL EDGE TYPE**



☐ Rounded



☐ Squared



☐ Pointed

**SELECT PONTIC DESIGN TYPE**



☐



☐



☐



☐





☐

☐ Perio treatment: Prepare tooth below gingival  
on tooth #(s) \_\_\_\_\_ by \_\_\_\_\_ mm

☐ Perio site healing: Prepare ovate socket  
on tooth #(s) \_\_\_\_\_ by \_\_\_\_\_ mm

Rx

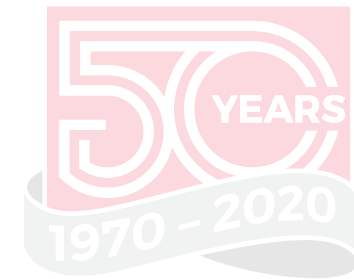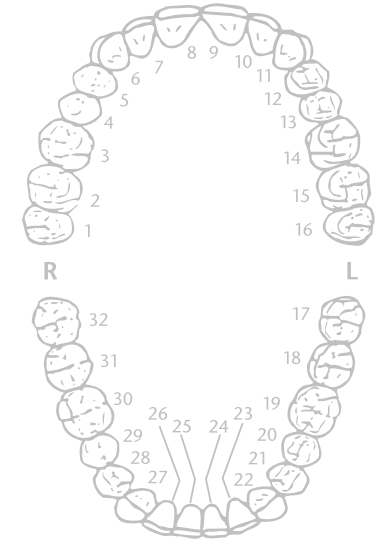

\*Standard unless specified otherwise

Signature \_\_\_\_\_ License # \_\_\_\_\_ Date \_\_\_\_\_

(see reverse for limited warranty details)


## TERMS AND WARRANTY INFORMATION

We honor VISA, MASTERCARD, AMEX and DISCOVER.

**TERMS:** Cost of collection of any account will be paid by the customer. All accounts are payable within 30 days of statement date. **Accounts not paid within the stated terms will be subject to COD status and a late charge of 2 percent of the unpaid balance.** Prices subject to change without notice. Rx must be enclosed with original case submission.

**NO-FAULT REMAKE POLICY:** Glidewell Laboratories is pleased to process all remakes or adjustments at no additional charge if requested within the warranty period and **accompanied by the return of the original appliance.**


**LIMITED WARRANTY/LIMITATION OF LIABILITY.** For warranty terms and conditions and limitation of liability, visit [glidewell dental.com/policies-and-warranties/](http://glidewell dental.com/policies-and-warranties/).



**All Restorations  
Made in the USA**


## PREPARATION GUIDELINES

### BIOTEMPS ANTERIOR




- A. 1 mm incisal reduction
- B. 0.8 mm middle third reduction
- C. Axial walls must be convergent (avoid undercuts)
- D. Preparation should be cut in three planes
- E. To achieve optimal impression quality, gingival retraction is necessary for preparations with subgingival or equigingival margins

### BIOTEMPS POSTERIOR

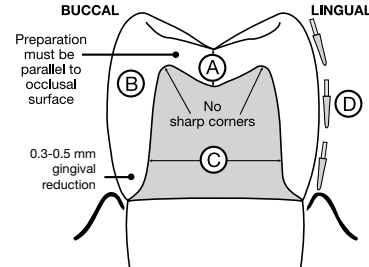


- A. 1 mm occlusal reduction
- B. 0.8 mm middle third reduction
- C. Axial walls must be convergent (avoid undercuts)
- D. Preparation should be cut in three planes
- E. To achieve optimal impression quality, gingival retraction is necessary for preparations with subgingival or equigingival margins

### BIOTEMPS VENEERS

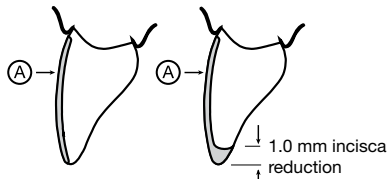

A. 0.3 to 1.0 mm labial reduction

### BIOTEMPS LABIAL OR 360° MARGIN

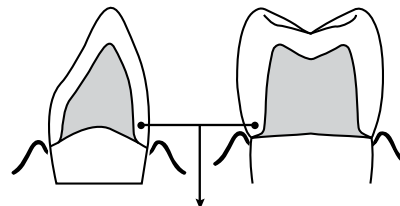

0.3-0.5 mm gingival reduction using rounded shoulder margin design


## IN-LAB WORKING TIMES

Please allow full working time for each product selected.  
Working times are NOT guaranteed and do NOT include weekends or holidays.


<b>BioTemps Provisionals</b> .....	5 days
w/ cast-metal frame or cast-metal reinforcement over implant .....	6 days
w/ cast-metal substructure .....	6 days
screw-retained over implant.....	6 days
extra cost for rush services .....	1 or 2 days
<b>Transition Crowns &amp; Bridges</b> .....	6 days
over implant.....	6 days
<b>Smile Transitions</b> .....	7 days

## BIOTEMPS RELINE INSTRUCTIONS


For best results, reline BioTemps Provisionals with a methyl methacrylate acrylic reline material (i.e., Jet® by Lang, Coldpac by Yates Motloid or Palavit® 55 by Heraeus Kulzer). Other reline materials should be avoided. However, if used, mechanical undercuts must be cut into the abutment shells for better retention of the reline material.

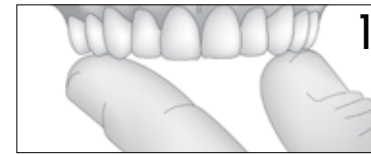


- Try in the restorations. If any adjustment is needed to seat the restoration, use a low-speed carbide or composite finishing bur.
- Rinse with water and dry completely.

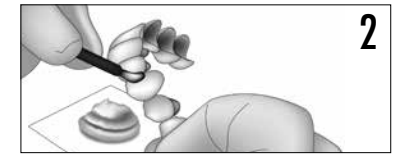

- Apply a thin layer of petroleum jelly to the outer surface of the restoration to prevent excess reline material from sticking.
- Reline provisionals by blocking out any undercuts on the preparations.

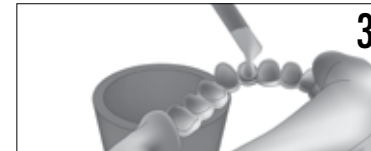

- Apply a minimal amount of reline material to the intaglio of the BioTemps. Use the mix tip to coat the inner walls with the material and evacuate any trapped air bubbles or voids.
- Do not allow the reline material to fully cure on the preparations due to heat generation, which may cause injury to the pulp.
- Gently work the BioTemps on and off the preps, allowing them to bench cure.

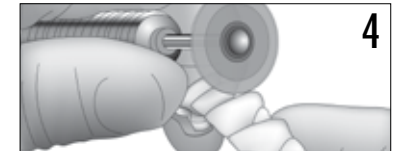

- Trim away any flash or excess acrylic using a plastic grinding disc.
- BioTemps can be polished with pumice and polishing paste or resealed with a light-cured glaze (e.g., Palaseal®, Heraeus Kulzer).
- Cement BioTemps using a non-eugenol temporary cement, like Zone™ by DUX Dental. If higher retention is needed, Neo-Temp® by Waterpik can be used.