




18551 Von Karman Ave. • Irvine, CA 92612
800-407-3262 • Fax 800-411-9722 • glidewell dental.com

Lab Name _____ Phone # _____
Acct. # _____ Patient Name _____
Address/Email _____
Deliver by 5 p.m. on _____

See Reverse for Working Times

Enclosed with case: ☐ Impressions ☐ Models ☐ Bite ☐ Photos ☐ Other: _____


Rx
☐ Coping(s)/substructure(s) ☐ Sintered only (stain & glaze)
☐ Build-up for porcelain support ☐ Finished completely
Indicate implant system _____ Implant diameter _____ mm

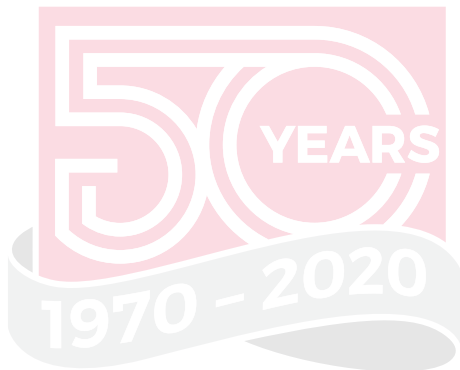


Signature _____

License # _____ Date _____

I verify that a signed prescription from a licensed dentist is on file for the restoration.
See reverse for limited warranty details.

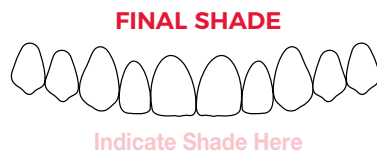

OCCUSAL STAINING
☐ None ☐ Light* ☐ Medium ☐ Dark

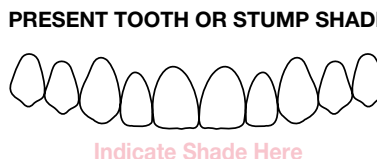



FINAL GINGIVAL SHADE
☐ G0 (Light) ☐ G1 (Standard)
☐ G3 (Med) ☐ G4 (Dark)



SELECT RESTORATION TYPE
☐ BruxZir Full-Strength Solid Zirconia (1,150 MPa)
☐ BruxZir Full-Strength Screw-Retained (w/Ti-Base)
☐ **NEW!** BruxZir Esthetic (870 MPa) (stump shade recommended for restorations less than 1.5 mm thick)
☐ **NEW!** BruxZir Esthetic Screw-Retained (w/Ti-Base)
☐ BruxZir Full-Arch Implant Prosthesis pre-stained and sintered (you stain, glaze and cement inserts)
☐ BruxZir Full-Arch Implant Prosthesis completely finished
☐ Full-Arch PMMA Provisional Implant Prosthesis completely finished
☐ IPS e.max (anterior) ☐ IPS e.max (posterior)
☐ IPS e.max Screw-Retained (w/Ti-Base)
☐ BioTemps ☐ Transition C&B ☐ Smile Transitions
Abutment #(s) _____ Pontic #(s) _____
Total Units _____
☐ Prismatic Clinical Zirconia ☐ Obsidian Fused to White Noble
☐ Obsidian Fused to Non-Precious ☐ Obsidian Fused to White High Noble



SELECT FINAL CUSTOM ABUTMENT
Choose Material : Choose Brand
☐ Titanium* ☐ Inclusive*
☐ Gold-Colored Titanium ☐ BIOMET 3i Encode
☐ Zirconia w/Ti-Base
☐ Gold Alloy
☐ Prepare existing abutment
See reverse for supported implant systems

PARALLEL ABUTMENTS
☐ No ☐ Yes (indicate which abutments will have restorations splinted together for insertion)

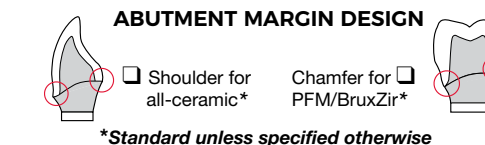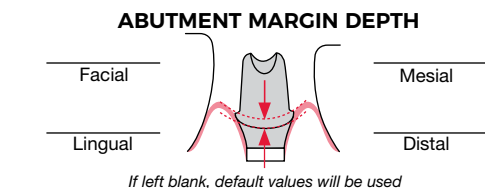


*Standard unless specified otherwise


SELECT BAR TYPE
INCLUSIVE IMPLANT BARS
☐ Locator CAD/CAM-Milled Bar
☐ Screw-Retained Hybrid Bar
☐ See reverse for supported implant systems

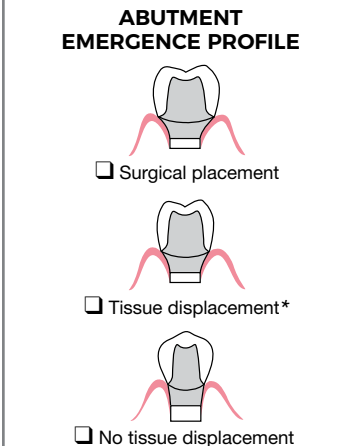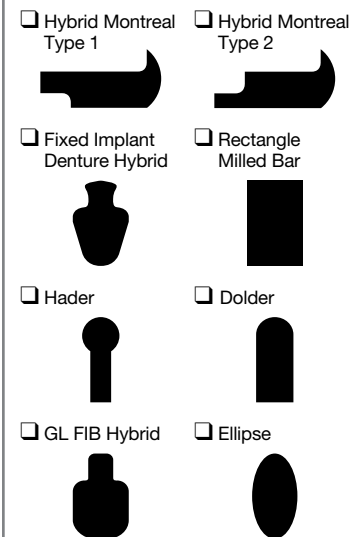

PLEASE COMPLETE THIS SECTION FOR IMPLANT BARS

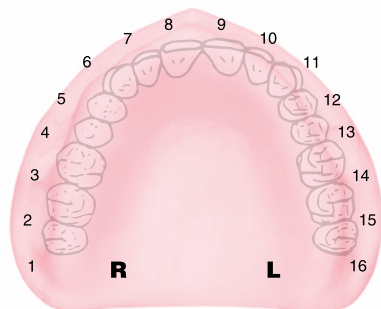

DISTANCE BETWEEN ANTERIOR AND POSTERIOR IMPLANTS: _____ mm
UPPER AP SPREAD X 1.5: _____ mm

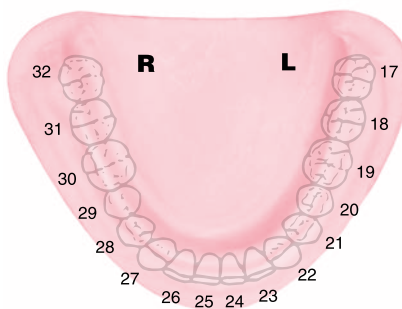

DISTANCE BETWEEN ANTERIOR AND POSTERIOR IMPLANTS: _____ mm
LOWER AP SPREAD X 1.5: _____ mm

IMPLANT WORKING TIMES

Please allow full working time for each product selected. Working times are NOT guaranteed and do NOT include weekends or holidays. Rush service available on most products but must be prescheduled (see below).

	<i>Days in Lab</i>
Inclusive Custom Abutments	8
Encode Custom Abutments	8
BruxZir restoration.....	5
IPS e.max restoration	5
Prismatik CZ restoration.....	5
Obsidian restoration	5
Full-cast restoration.....	5
BruxZir Screw-Retained crown	8
IPS e.max Screw-Retained crown.....	8
Obsidian Screw-Retained crown.....	8
BruxZir Full-Arch Implant Prosthesis pre-stained	6
BruxZir Full-Arch Implant Prosthesis finished	8
PMMA Full-Arch Implant Prosthesis finished.....	6
Locator CAD/CAD-Milled Bar.....	7
Screw-Retained Hybrid Bar.....	8
BioTemps.....	5
BioTemps cement over implant/cast-metal substructure/screw-retained	6
Transition Crowns & Bridges	6
Smile Transitions	7

All rush cases must be prescheduled by calling 800-944-7874 before the case is shipped.
Time of pickup and delivery may affect turnaround time.

TERMS AND WARRANTY INFORMATION



**All Restorations
Made in the USA**

We honor VISA, MASTERCARD, AMEX and DISCOVER.

TERMS: Cost of collection of any account will be paid by the customer. All accounts are payable within 30 days of statement date. **Accounts not paid within the stated terms will be subject to COD status and a late charge of 2 percent of the unpaid balance.** Prices subject to change without notice. Rx must be enclosed with original case submission.

NO-FAULT REMAKE POLICY: Glidewell Laboratories is pleased to process all remakes or adjustments at no additional charge if requested within the warranty period and accompanied by the return of the original appliance.

LIMITED WARRANTY/LIMITATION OF LIABILITY. For warranty terms and conditions and limitation of liability, visit glidewelldental.com/policies-and-warranties.

CUSTOM ABUTMENTS AND SCREW-RETAINED CROWNS ARE COMPATIBLE WITH THE FOLLOWING IMPLANT SYSTEMS

BIOMET 3i™ Certain®	CAMLOG® SCREW-LINE™	Dentium® Implantium®† SimpleLine® II† SuperLine®†
DENTSPLY Implants ANKYLOS® C/X* ASTRA TECH Implant System®* ASTRA TECH Implant System® EV*	Glidewell Direct Hahn™ Tapered Implant System† Inclusive® Tapered Implant System*	HIOSS® HG System*
Keystone Dental PrimaConnex®†	MegaGen AnyRidge® Implant System*	Neoss® Neoss® Implant System†
Straumann® Bone Level* Tissue Level*	Sweden & Martina Premium† Shelta†	Nobel Biocare Brånemark System® RP* NobelActive®* NobelReplace®*
		Zimmer Dental Screw-Vent®*

THE BRUXZIR® FULL-ARCH IMPLANT PROSTHESIS IS COMPATIBLE WITH THE FOLLOWING IMPLANT SYSTEMS

BIOMET 3i™ Certain®	CAMLOG® SCREW-LINE	DENTSPLY Implants ANKYLOS® C/X ASTRA TECH Implant System® ASTRA TECH Implant System® EV
Glidewell Direct Hahn™ Tapered Implant System Inclusive® Tapered Implant System	HIOSS® HG System	MegaGen AnyRidge® Implant System
Nobel Biocare Brånemark System® RP NobelActive® NobelReplace®	Straumann® Bone Level Tissue Level	Sweden & Martina Premium Shelta
		Zimmer Dental Screw-Vent®

*Manufactured using Inclusive® components. †Manufactured using original equipment manufacturer (OEM) components.
Inclusive is a registered trademark of Prismatik Dentalcraft, Inc. Hahn Tapered Implant is a trademark of Prismatik Dentalcraft, Inc.
All other trademarks are property of their respective owners. For Dentium implant systems, only titanium custom abutments are available.
For the BruxZir Full-Arch Implant Prosthesis, prices vary for Sweden & Martina.